


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031120\
Data File : VU037152.D
Acq On : 10 Mar 2020 14:34
Operator : JC/MD
Sample : BFB01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Mar 12 01:55:55 2020

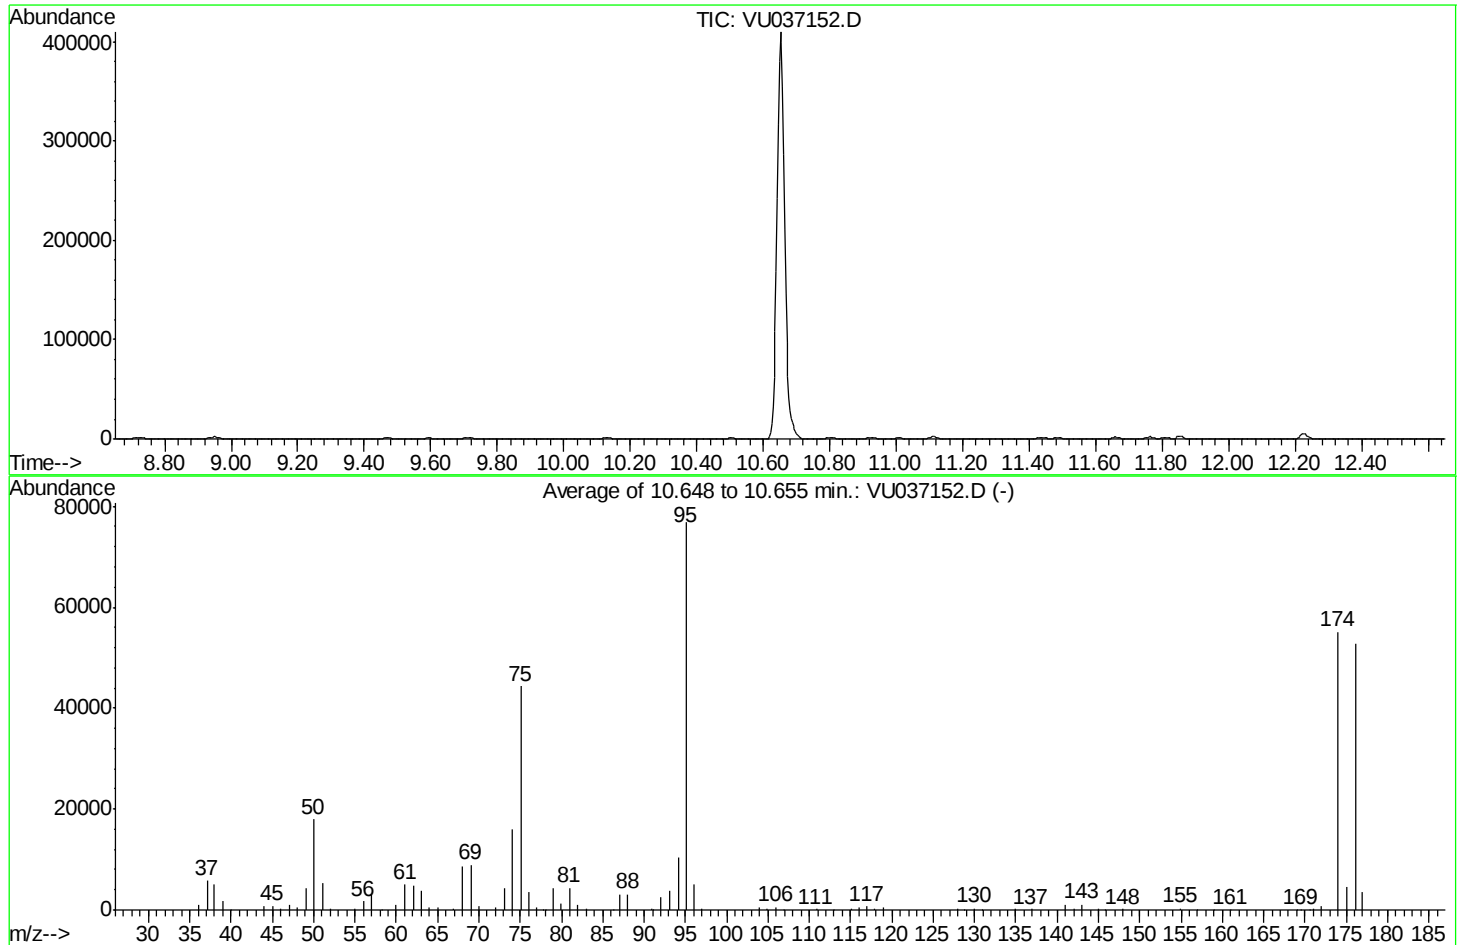

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	17901	PASS
75	95	30	80	57.7	44296	PASS
95	95	100	100	100.0	76832	PASS
96	95	5	9	6.8	5201	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.8	55186	PASS
175	174	5	9	8.1	4496	PASS
176	174	95	101	95.6	52762	PASS
177	176	5	9	6.6	3493	PASS

m/z	Abundance
36.00	971.0
37.10	5380.0
38.00	4958.0
39.10	1848.0
40.00	121.0
44.00	961.0
45.00	853.0
46.00	134.0
47.00	846.0
48.00	541.0
49.00	4248.0
50.00	17024.0
51.00	5189.0
52.00	278.0
54.90	236.0
56.00	1667.0
57.10	2928.0
58.20	148.0
60.00	1057.0
61.00	4927.0
62.10	4652.0
63.00	3715.0
64.00	599.0
65.10	577.0
67.00	264.0
68.00	8409.0
69.10	8918.0
70.00	683.0
72.00	557.0
73.00	4255.0
74.10	15337.0
75.10	42904.0
76.00	3522.0
77.00	474.0
78.10	284.0
79.00	4056.0
79.90	1245.0
81.00	4176.0
82.00	1041.0
83.10	167.0
86.20	165.0
87.00	2878.0
88.00	2879.0
90.80	330.0
91.10	321.0
92.00	2552.0
93.00	3592.0
94.10	10080.0
95.10	73800.0
96.10	5186.0
97.00	148.0
103.90	451.0
104.90	167.0
106.00	498.0
106.90	130.0
110.80	159.0
112.90	105.0
115.00	133.0
115.90	377.0
117.00	602.0
117.90	329.0
118.90	621.0
127.80	304.0
130.00	256.0
130.90	134.0
135.00	128.0
136.90	171.0
141.00	1065.0
142.00	208.0
143.00	1079.0
145.00	139.0
145.90	130.0
148.00	146.0
154.90	260.0
157.00	109.0
158.90	116.0
169.50	110.0
170.90	193.0
172.00	765.0
174.00	51224.0
175.00	4443.0
176.10	49400.0
177.00	3519.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	1047.0
37.10	5977.0
38.00	5228.0
39.10	1810.0
40.00	129.0
44.00	936.0
45.00	889.0
46.10	156.0
47.10	937.0
48.10	601.0
49.00	4473.0
50.00	18536.0
51.10	5549.0
52.00	311.0
54.90	270.0
56.00	1760.0
57.10	3174.0
58.20	120.0
60.00	1150.0
61.00	5244.0
62.10	5032.0
63.00	3912.0
64.00	628.0
65.10	601.0
66.90	257.0
68.00	8802.0
69.00	9276.0
70.00	714.0
72.10	598.0
73.00	4382.0
74.00	16664.0
75.10	45752.0
76.10	3751.0
77.00	558.0
79.00	4376.0
79.90	1409.0
81.00	4585.0
82.00	1083.0
83.00	181.0
86.20	161.0
87.00	3216.0
88.00	3289.0
90.80	385.0
92.00	2666.0
93.10	3857.0
94.10	10798.0
95.10	79504.0
96.10	5386.0
97.00	167.0
103.90	535.0
104.90	183.0
106.00	557.0
106.90	124.0
110.90	139.0
112.80	119.0
115.10	155.0
115.90	454.0
117.00	687.0
117.90	378.0
119.00	667.0
127.90	272.0
128.80	145.0
130.00	300.0
130.90	147.0
135.00	147.0
136.90	205.0
141.00	1139.0
142.00	200.0
143.00	1140.0
145.00	159.0
145.80	125.0
148.00	198.0
154.90	271.0
156.90	102.0
158.90	116.0
161.00	100.0
169.10	103.0
169.50	105.0
171.00	188.0
172.00	865.0
174.00	56816.0
175.10	4644.0
176.10	54400.0
177.00	3612.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	1013.0
37.10	5909.0
38.00	4931.0
39.00	1676.0
40.00	126.0
44.00	882.0
45.00	840.0
46.10	167.0
47.10	975.0
48.00	604.0
49.10	4259.0
50.00	18144.0
51.10	5324.0
52.10	286.0
55.00	272.0
56.00	1641.0
57.00	3022.0
60.00	1119.0
61.10	4898.0
62.10	5020.0
63.00	3771.0
64.00	557.0
65.10	584.0
66.90	204.0
68.00	8448.0
69.00	8452.0
70.00	695.0
72.10	606.0
73.10	4167.0
74.00	16098.0
75.10	44232.0
76.10	3615.0
77.00	556.0
77.80	227.0
79.00	4408.0
80.00	1329.0
81.00	4504.0
81.90	1074.0
83.00	194.0
87.00	3103.0
88.00	3185.0
90.90	429.0
92.00	2552.0
93.10	3706.0
94.10	10583.0
95.10	77192.0
96.10	5031.0
97.00	184.0
103.90	516.0
104.90	160.0
106.00	556.0
106.90	106.0
110.90	125.0
112.80	137.0
115.10	136.0
116.00	455.0
117.00	689.0
117.90	415.0
118.90	608.0
128.00	261.0
128.80	196.0
130.00	292.0
131.00	126.0
134.90	159.0
136.90	217.0
141.00	1041.0
142.10	170.0
143.00	1046.0
145.00	158.0
145.70	116.0
148.00	203.0
155.00	251.0
156.90	104.0
158.90	100.0
169.00	103.0
170.60	126.0
171.10	145.0
172.00	815.0
174.00	57520.0
175.10	4401.0
176.10	54488.0
177.00	3348.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
44.10	204.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01