


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031120\
 Data File : VU037159.D
 Acq On : 11 Mar 2020 10:17
 Operator : JC/MD
 Sample : BFB02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB02

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Mar 12 01:55:55 2020

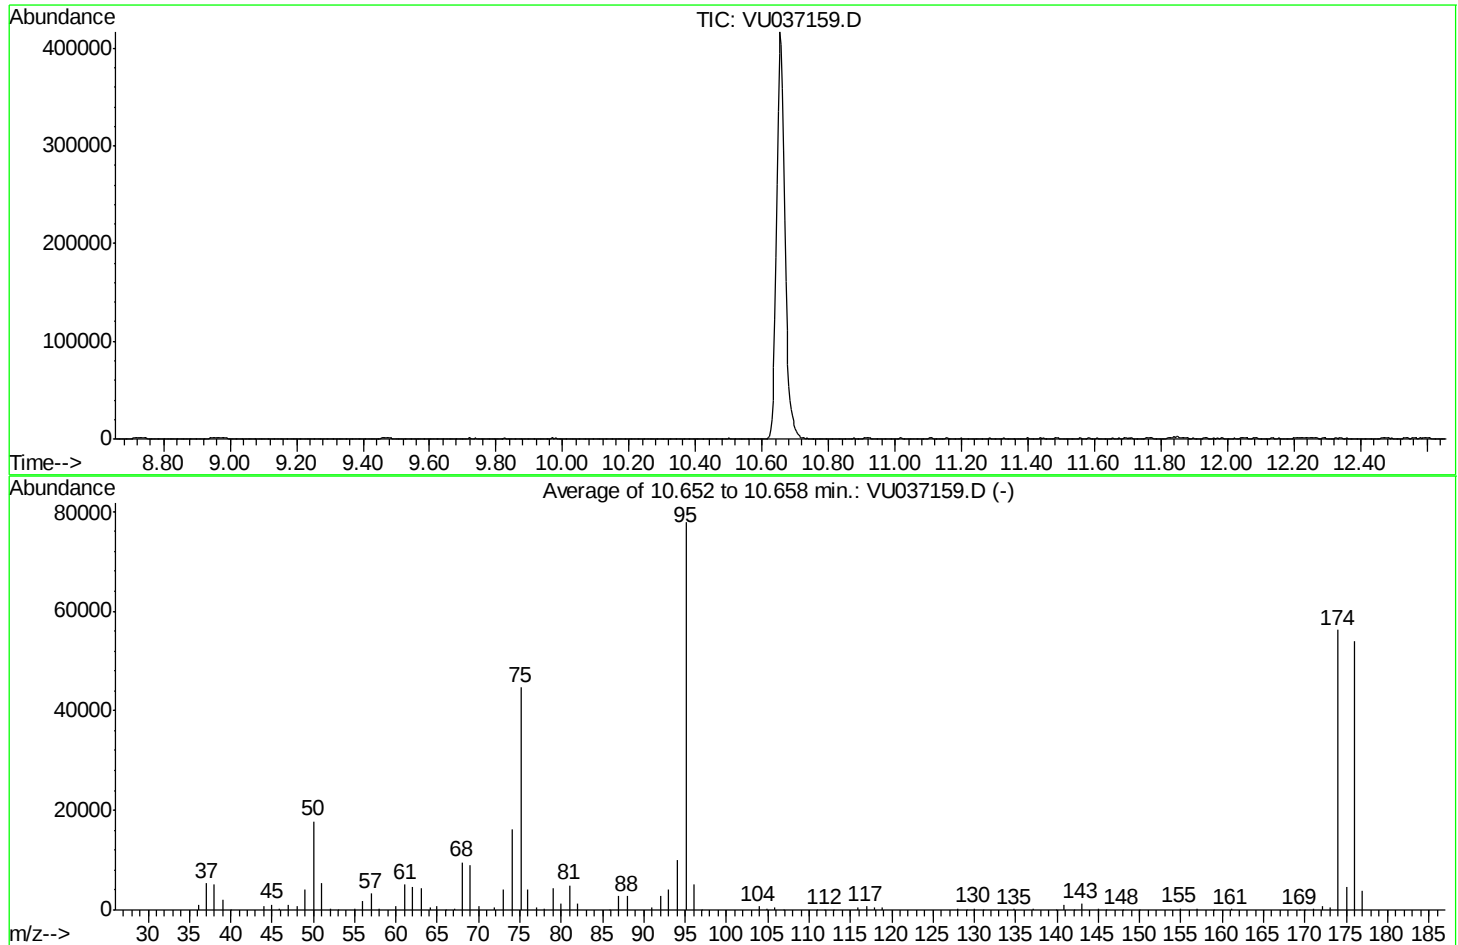

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	17789	PASS
75	95	30	80	57.4	44637	PASS
95	95	100	100	100.0	77818	PASS
96	95	5	9	6.7	5219	PASS
173	174	0.00	2	0.8	469	PASS
174	95	50	120	72.2	56197	PASS
175	174	5	9	8.4	4726	PASS
176	174	95	101	96.2	54085	PASS
177	176	5	9	6.9	3740	PASS

m/z	Abundance
36.10	914.0
37.10	5286.0
38.00	5229.0
39.00	2183.0
40.00	163.0
44.00	1082.0
45.00	989.0
45.90	175.0
47.00	1066.0
48.00	794.0
49.00	4099.0
50.00	17752.0
51.00	5568.0
52.10	246.0
53.00	130.0
55.00	310.0
56.00	1832.0
57.00	3050.0
57.90	127.0
59.90	938.0
61.10	4852.0
62.10	4732.0
63.00	4325.0
64.10	612.0
65.00	739.0
67.00	252.0
68.00	9574.0
69.00	9281.0
70.00	711.0
72.00	487.0
73.00	3842.0
74.10	15906.0
75.10	43656.0
76.00	4215.0
76.90	423.0
77.90	317.0
79.00	4416.0
79.90	1387.0
81.00	4851.0
81.90	1250.0
87.00	2656.0
88.00	2669.0
90.90	450.0
92.00	2588.0
93.00	3773.0
94.10	9840.0
95.10	76280.0
96.10	5154.0
97.00	176.0
103.90	724.0
104.90	153.0
105.90	606.0
106.80	121.0
115.90	479.0
116.90	759.0
118.00	393.0
118.90	556.0
127.80	258.0
130.00	370.0
131.00	118.0
134.90	250.0
137.10	188.0
140.90	1073.0
143.00	1245.0
145.00	206.0
146.00	116.0
149.90	102.0
154.90	276.0
156.90	292.0
161.10	114.0
169.40	112.0
171.00	245.0
172.10	753.0
173.00	1407.0
174.00	52704.0
175.10	4597.0
176.00	50752.0
177.00	3637.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.00	942.0
37.10	5411.0
38.00	5231.0
39.00	2289.0
40.00	175.0
44.00	1024.0
45.00	1108.0
46.00	170.0
47.00	1030.0
48.00	860.0
49.00	4313.0
50.00	18328.0
51.00	5593.0
52.10	312.0
54.90	277.0
56.00	1794.0
57.00	3414.0
57.90	185.0
59.90	884.0
61.10	5200.0
62.00	4783.0
63.00	4668.0
64.10	627.0
65.00	696.0
68.00	9891.0
69.00	9347.0
70.10	714.0
72.00	474.0
73.00	4250.0
74.10	16624.0
75.10	45992.0
76.00	4473.0
77.00	459.0
78.00	352.0
78.90	4661.0
79.90	1435.0
81.00	5032.0
81.90	1292.0
87.00	2883.0
88.00	2871.0
91.00	516.0
92.00	2942.0
93.00	4123.0
94.10	10407.0
95.10	80312.0
96.10	5311.0
97.00	126.0
104.00	718.0
104.90	177.0
105.90	547.0
106.90	145.0
111.00	117.0
111.90	132.0
115.90	485.0
116.90	780.0
118.00	420.0
118.90	628.0
127.90	254.0
129.00	108.0
129.90	333.0
131.00	142.0
134.80	193.0
137.10	203.0
140.90	1040.0
142.00	122.0
143.00	1343.0
145.00	209.0
146.00	113.0
147.90	100.0
149.90	112.0
154.90	412.0
156.90	260.0
158.90	123.0
161.10	206.0
169.40	105.0
170.00	128.0
171.00	231.0
172.10	847.0
174.00	57864.0
175.00	4875.0
176.10	55720.0
177.00	3830.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

m/z	Abundance
36.00	1065.0
37.10	5256.0
38.00	4633.0
39.00	1977.0
40.10	184.0
44.10	1061.0
45.00	1051.0
46.00	162.0
46.90	806.0
48.00	722.0
49.00	4274.0
50.10	17288.0
51.00	5093.0
52.10	355.0
54.90	273.0
56.00	1635.0
57.00	3282.0
57.90	191.0
60.00	760.0
61.10	5067.0
62.00	4369.0
63.00	4523.0
64.10	551.0
65.00	685.0
66.00	107.0
67.10	298.0
68.00	9325.0
69.00	8653.0
70.10	657.0
71.90	474.0
73.10	4440.0
74.10	15823.0
75.10	44264.0
76.00	4023.0
77.00	520.0
78.10	358.0
78.90	4414.0
79.90	1370.0
81.00	4790.0
81.90	1277.0
85.80	104.0
87.00	2737.0
88.00	2749.0
91.10	474.0
92.00	3001.0
93.00	4111.0
94.10	10185.0
95.10	76864.0
96.10	5194.0
97.10	103.0
104.00	654.0
104.90	144.0
105.90	448.0
107.00	153.0
111.00	136.0
111.90	136.0
112.90	134.0
115.90	411.0
116.90	738.0
117.90	396.0
118.80	620.0
128.00	290.0
129.00	112.0
129.90	294.0
131.00	120.0
134.80	159.0
137.00	174.0
139.90	131.0
140.90	943.0
142.00	111.0
143.00	1222.0
145.00	169.0
147.90	155.0
154.90	418.0
157.00	196.0
158.90	140.0
161.10	254.0
170.00	148.0
171.10	204.0
172.10	930.0
174.00	58024.0
175.00	4706.0
176.10	55784.0
177.00	3753.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02

Scan 2883 (10.610 min): VU037159.D
BFB02

m/z	Abundance
40.00	148.0
44.00	303.0

Instrument :
MSVOA_U
ClientSampleId :
BFB02