

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031121\
 Data File : VU042558.D
 Acq On : 11 Mar 2021 10:50
 Operator : SY/MD
 Sample : VU0311WBL07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK29

Quant Time: Mar 11 11:15:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Mar 10 06:46:59 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.124	96	17214	1.00	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.642	95	6471	0.85	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.00%	
68) 1,2-Dichlorobenzene-d4	12.205	152	6729	0.86	ug/l	0.00
Spiked Amount 1.000			Recovery	=	86.00%	
Target Compounds						
15) Methylene Chloride	3.057	84	1294	0.25	ug/l	# 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031121\
Data File : VU042558.D
Acq On : 11 Mar 2021 10:50
Operator : SY/MD
Sample : VU0311WBL07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK29

Quant Time: Mar 11 11:15:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U030921DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Mar 10 06:46:59 2021
Response via : Initial Calibration

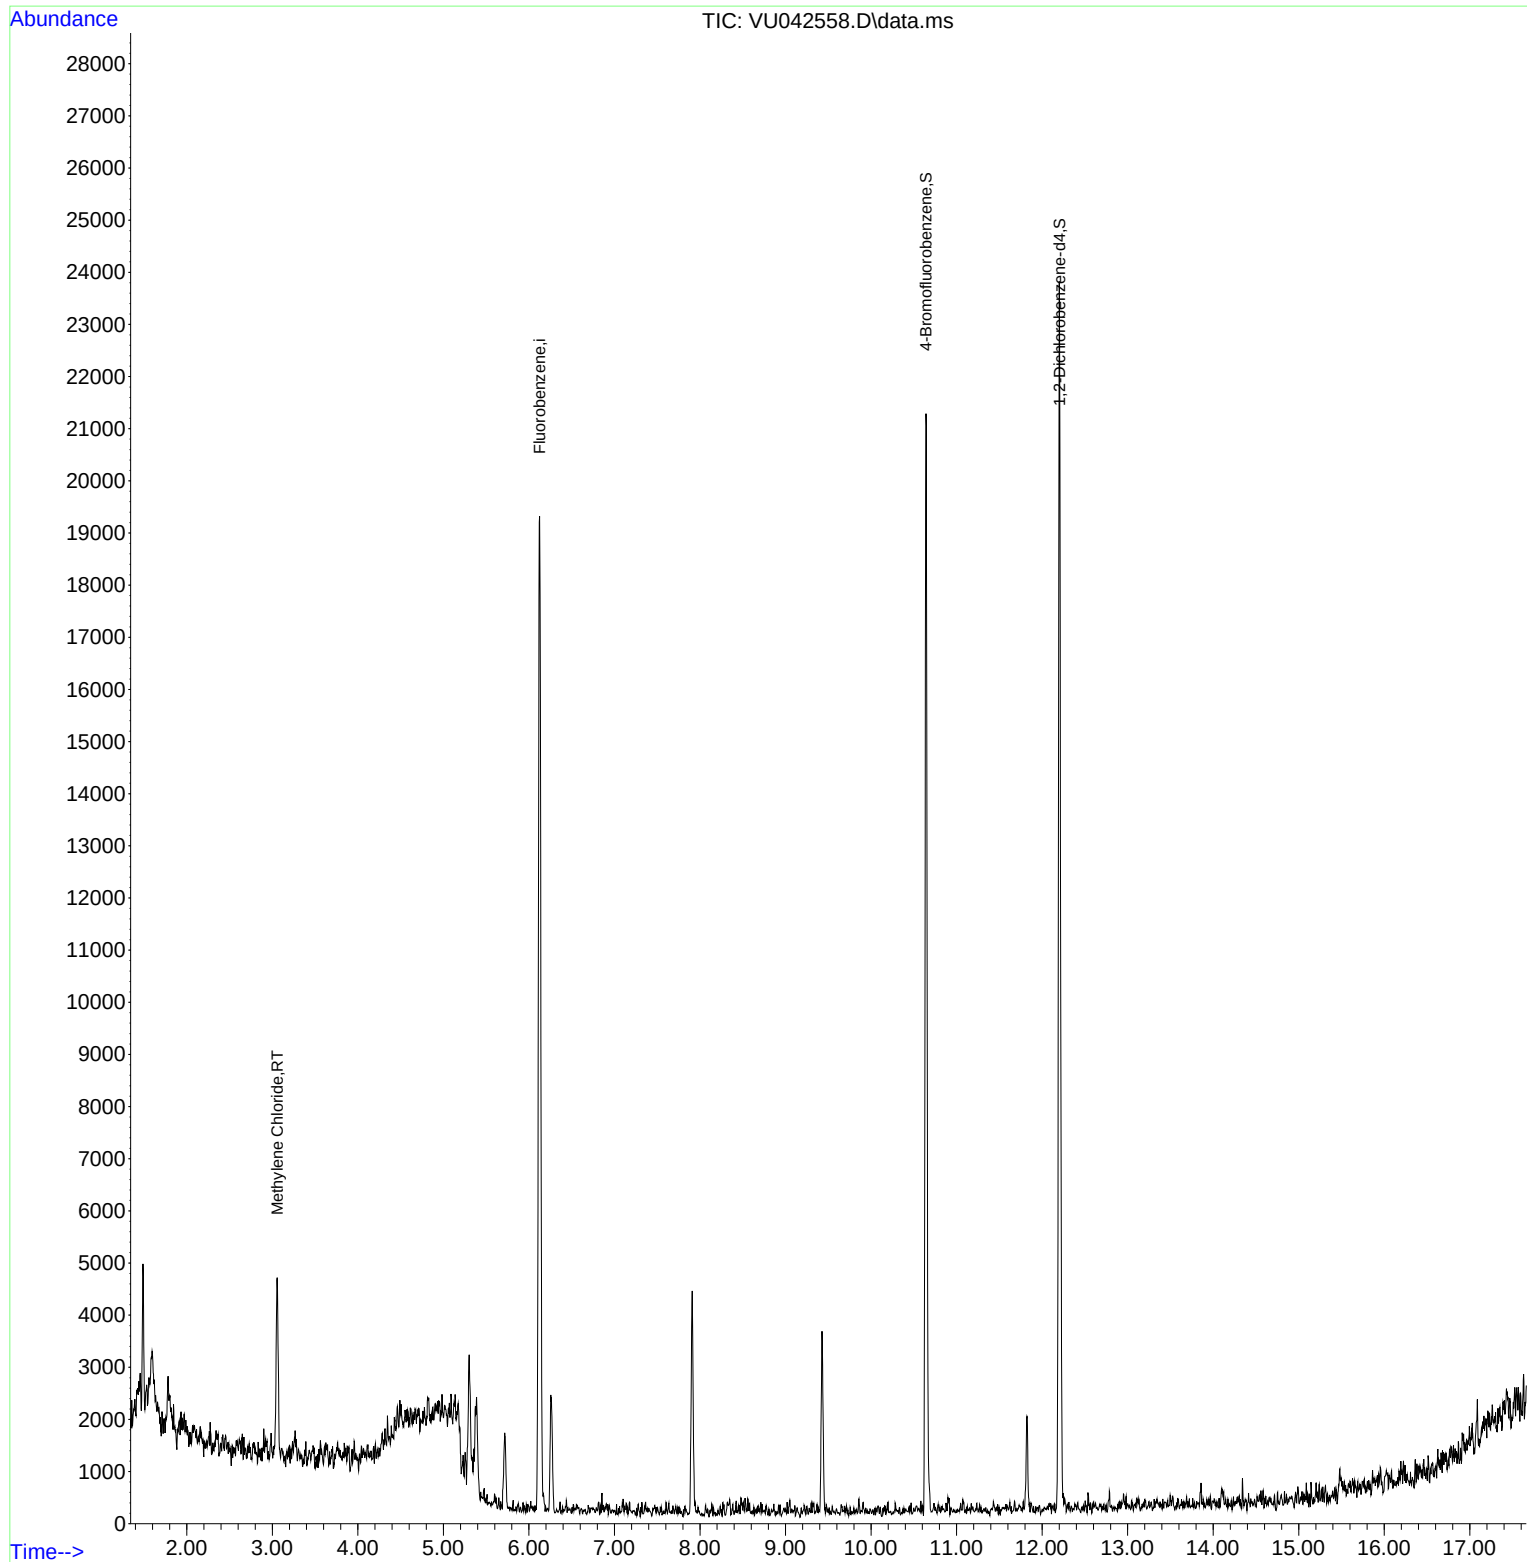




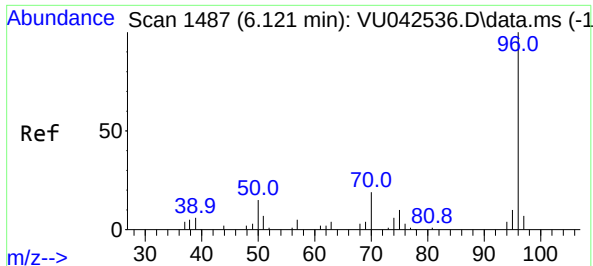


#1
Fluorobenzene
Concen: 1.00 ug/l
RT: 6.124 min Scan# 1488
Delta R.T. 0.003 min
Lab File: VU042558.D
Acq: 11 Mar 2021 10:50

Instrument :
MSVOA_U
ClientSampleId :
VBLK29

Tgt Ion: 96 Resp: 17214




Ion	Ratio	Lower	Upper
96	100		
70	19.7	16.3	24.5
95	9.3	7.0	10.4
97	6.6	0.0	0.0

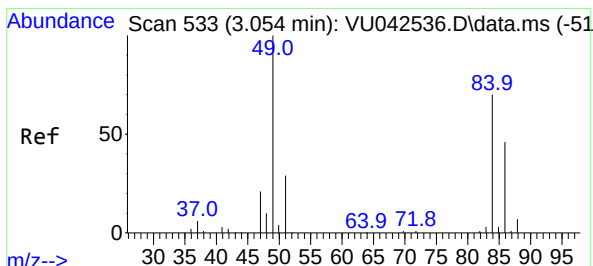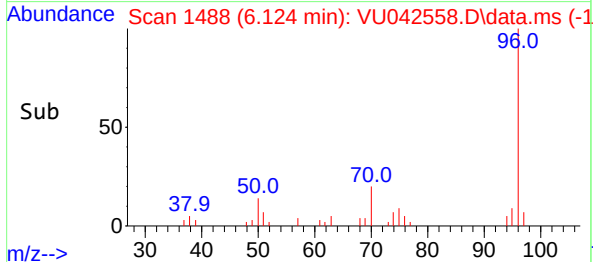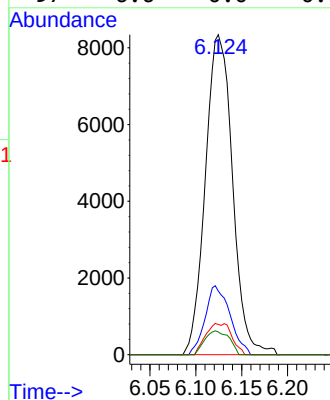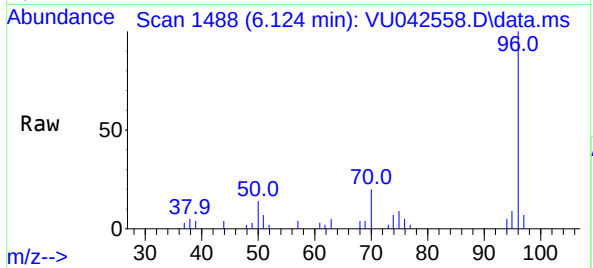


#15
Methylene Chloride
Concen: 0.25 ug/l
RT: 3.057 min Scan# 534
Delta R.T. 0.003 min
Lab File: VU042558.D
Acq: 11 Mar 2021 10:50

Tgt Ion: 84 Resp: 1294

Ion	Ratio	Lower	Upper
84	100		
49	114.6	114.6	172.0
51	43.7	0.0	83.0
86	49.9	52.3	78.5


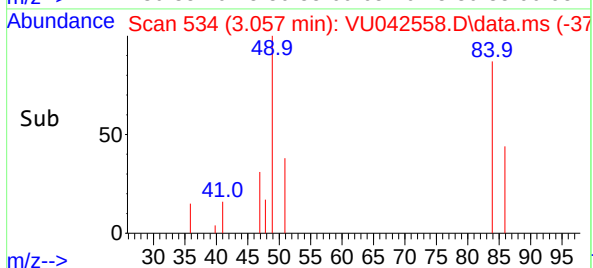
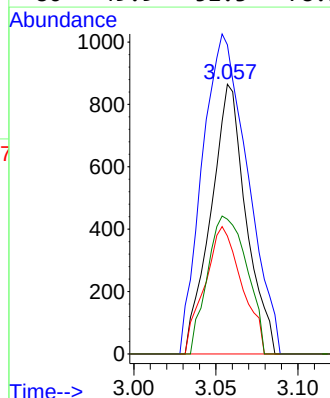
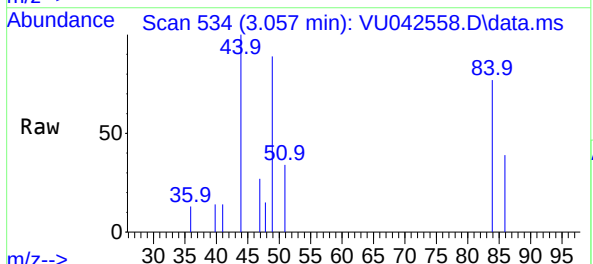


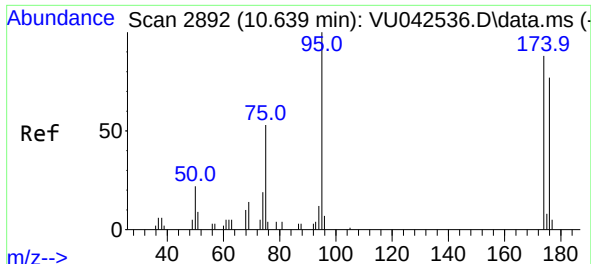

#57
4-Bromofluorobenzene
Concen: 0.85 ug/l
RT: 10.642 min Scan# 2893
Delta R.T. 0.003 min
Lab File: VU042558.D
Acq: 11 Mar 2021 10:50

Instrument :
MSVOA_U
ClientSampleId :
VBLK29

Tgt Ion: 95 Resp: 6471
Ion Ratio Lower Upper
95 100
174 94.1 73.1 109.7
176 87.2 63.4 95.2

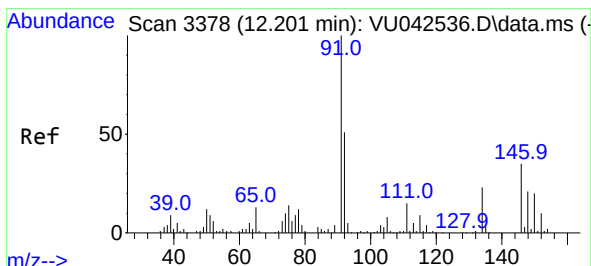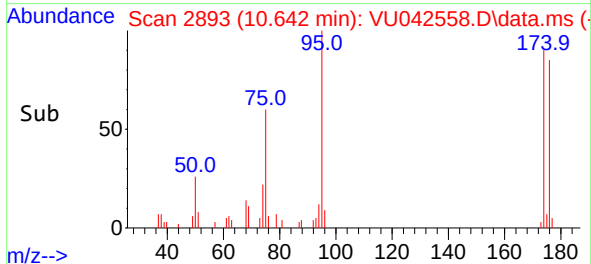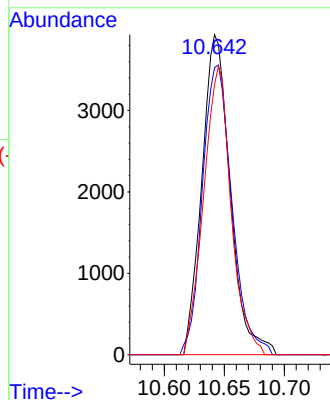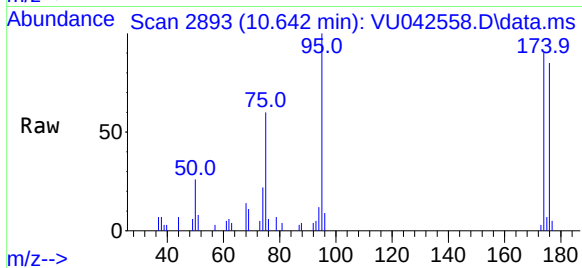

#68
1,2-Dichlorobenzene-d4
Concen: 0.86 ug/l
RT: 12.205 min Scan# 3379
Delta R.T. 0.003 min
Lab File: VU042558.D
Acq: 11 Mar 2021 10:50

Tgt Ion:152 Resp: 6729
Ion Ratio Lower Upper
152 100
115 58.1 0.0 266.0
150 146.3 0.0 657.2

