




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
Data File : VU029949.D
Acq On : 10 Mar 2019 15:15
Operator : JC/SP
Sample : K1818-12ME
Misc : 5.80g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0R2ME

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:48:06 AM

Quant Time: Mar 11 07:14:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 07:10:15 2019
Response via : Initial Calibration

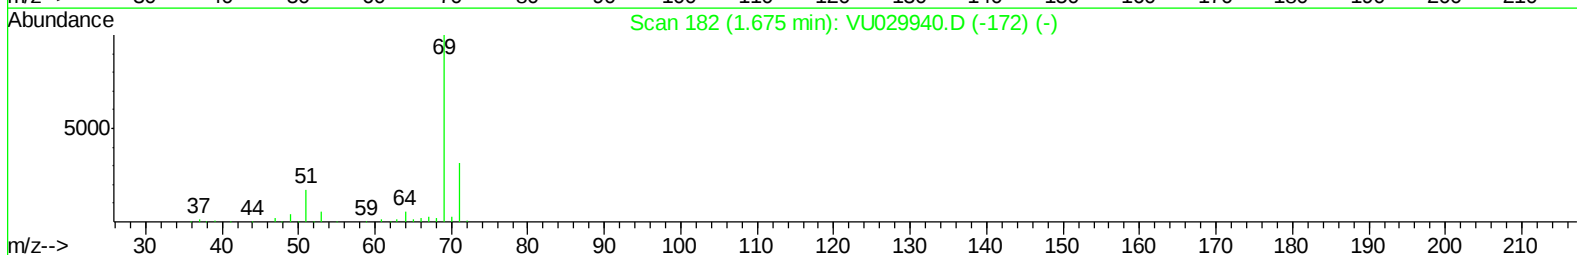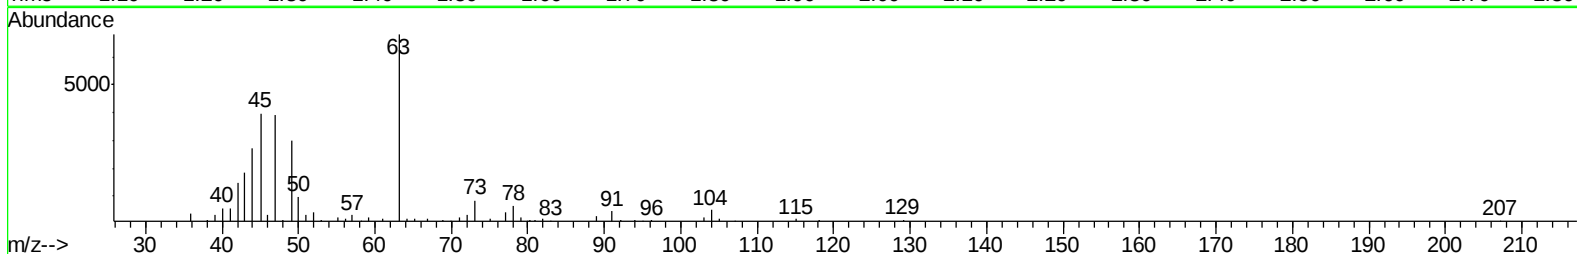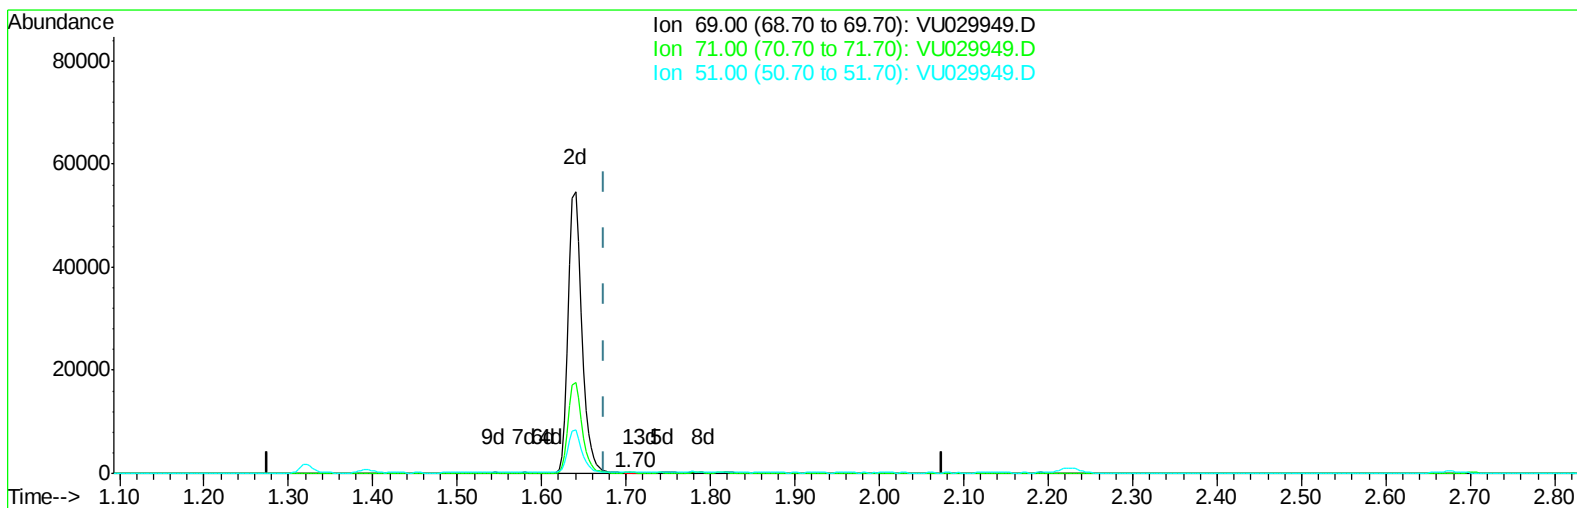

TIC: VU029949.D

(7) Chloroethane-d5 (S)

1.704min (+0.029) 0.05ug/L

response 158

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	124.05#
51.00	24.10	90.51#
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
Data File : VU029949.D
Acq On : 10 Mar 2019 15:15
Operator : JC/SP
Sample : K1818-12ME
Misc : 5.80g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0R2ME

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:48:06 AM

Quant Time: Mar 11 07:14:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 07:10:15 2019
Response via : Initial Calibration

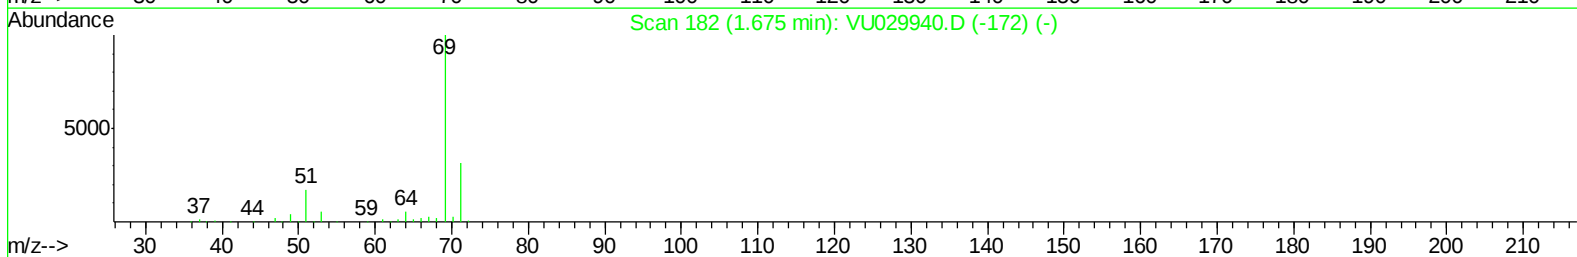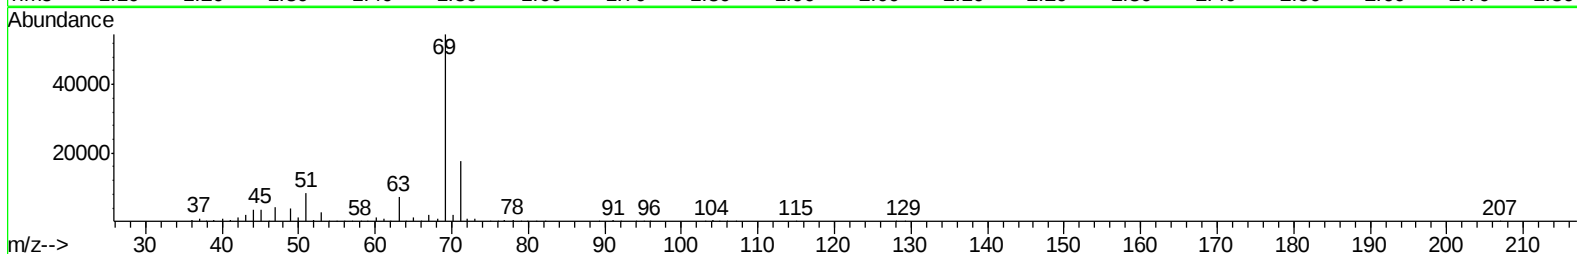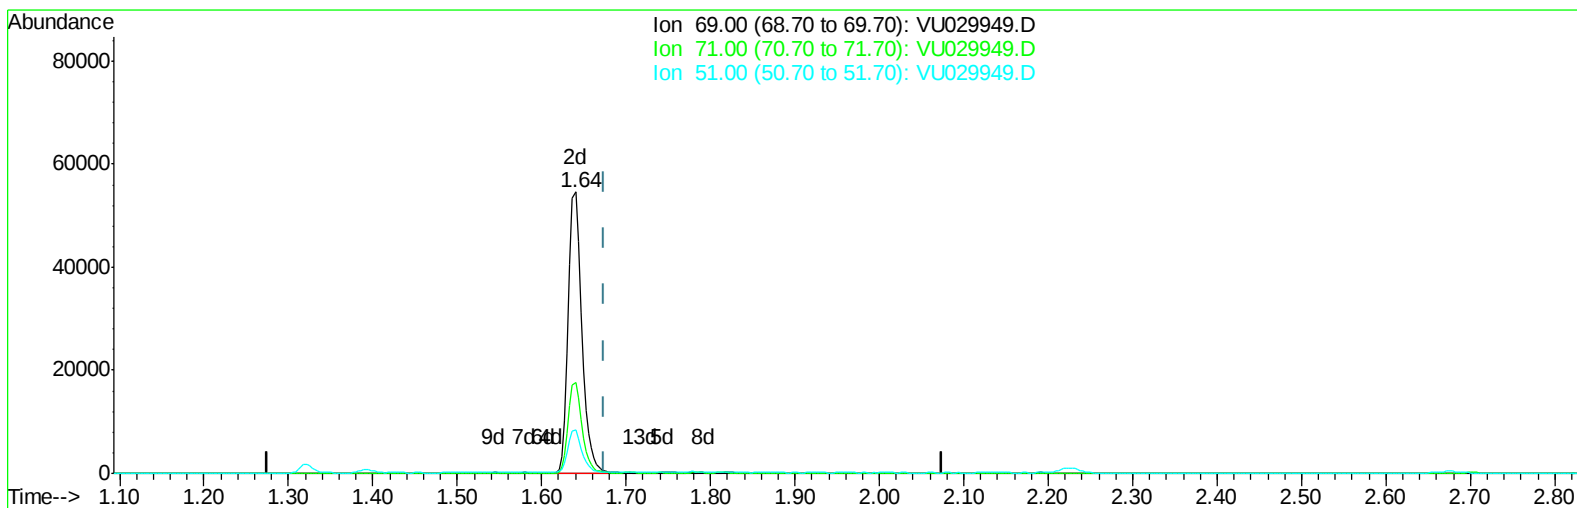

TIC: VU029949.D

(7) Chloroethane-d5 (S)

1.640min (-0.036) 20.17ug/L m

response 60554

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	0.32#
51.00	24.10	0.24#
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
 Data File : VU029949.D
 Acq On : 10 Mar 2019 15:15
 Operator : JC/SP
 Sample : K1818-12ME
 Misc : 5.80g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0R2ME

Manual Integrations
 APPROVED

MMDadoda
 3/11/2019 11:48:06 AM

Quant Time: Mar 11 07:14:33 2019
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 11 07:10:15 2019
 Response via : Initial Calibration

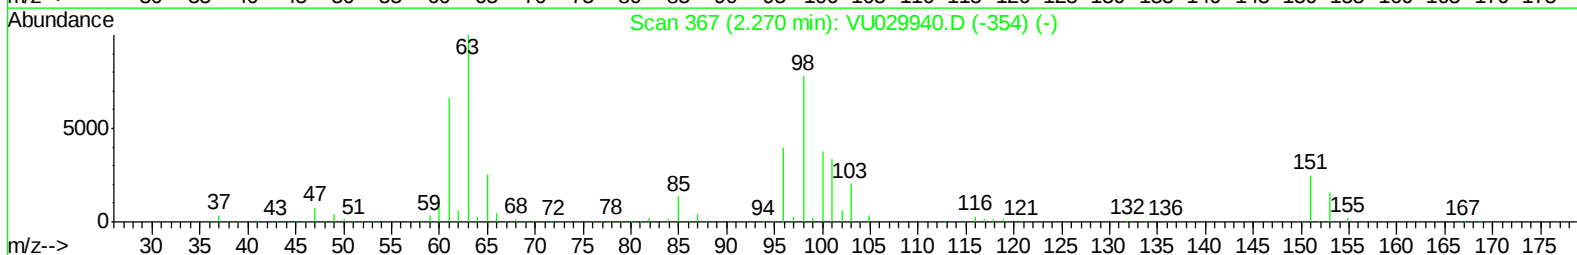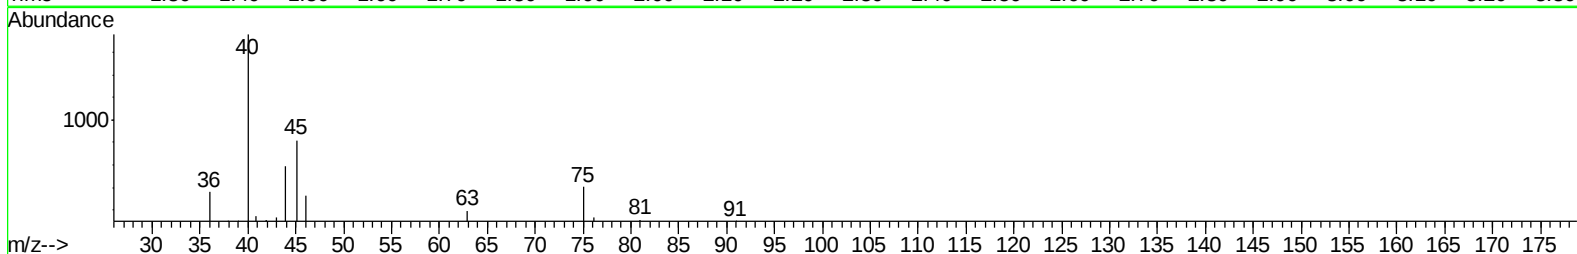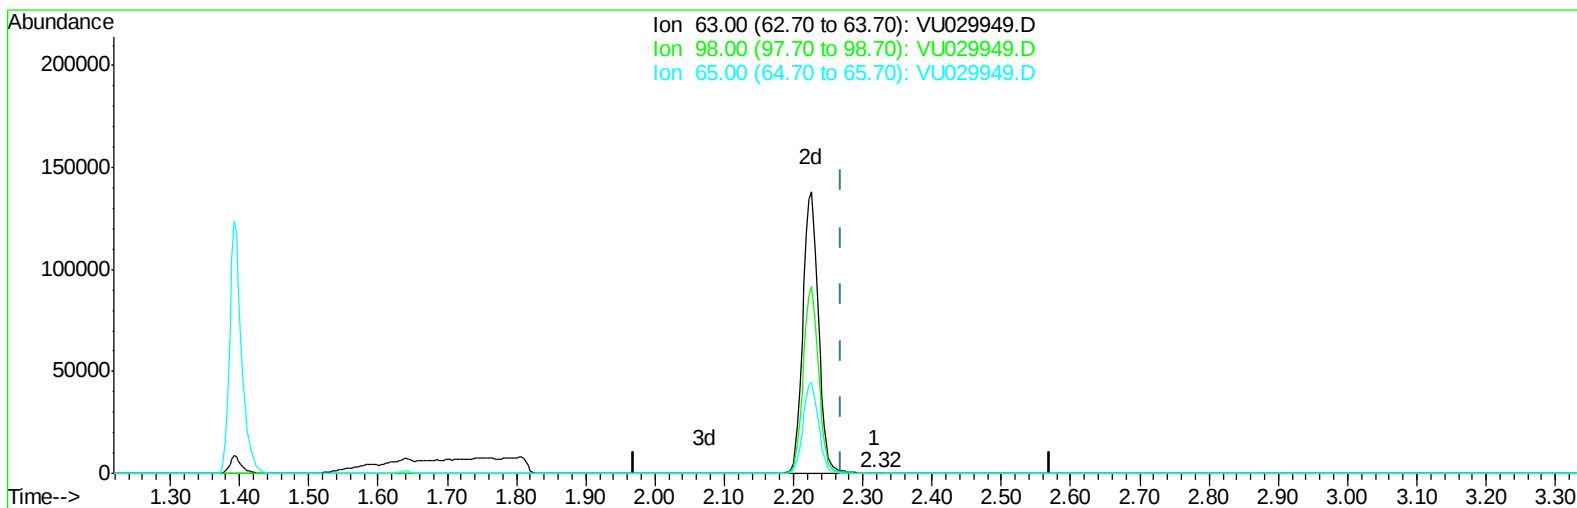

TIC: VU029949.D

(11) 1,1-Dichloroethene-d2 (S)

2.318min (+0.048) 0.03ug/L

response 185

Ion	Exp%	Act%
63.00	100	100
98.00	82.90	83.78
65.00	23.60	0.00#
0.00	0.00	0.00




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
 Data File : VU029949.D
 Acq On : 10 Mar 2019 15:15
 Operator : JC/SP
 Sample : K1818-12ME
 Misc : 5.80g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0R2ME

Manual Integrations
 APPROVED

MMDadoda
 3/11/2019 11:48:06 AM

Quant Time: Mar 11 07:14:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 11 07:10:15 2019
 Response via : Initial Calibration

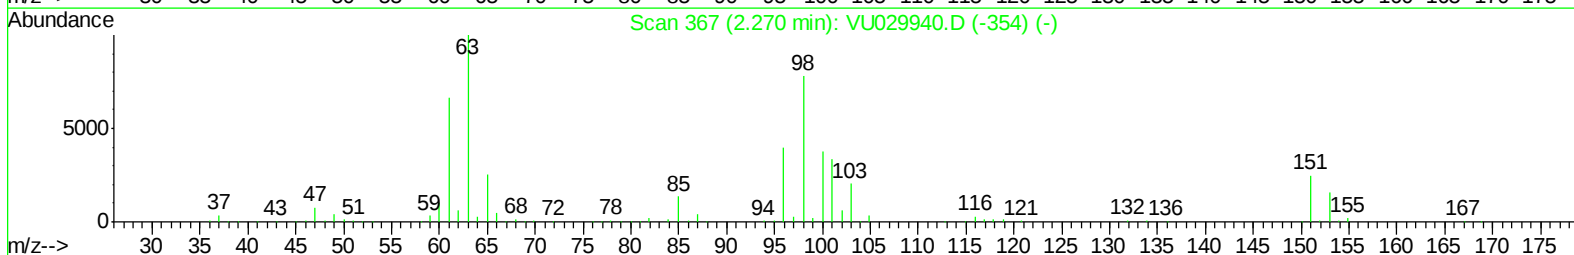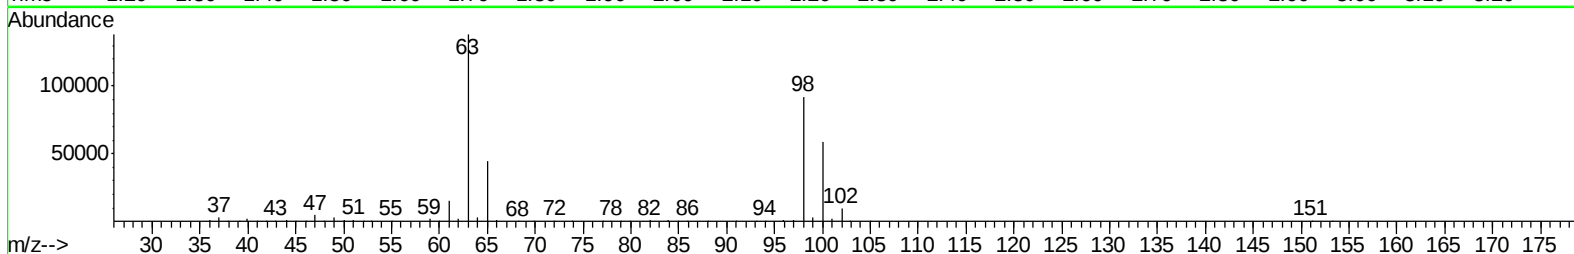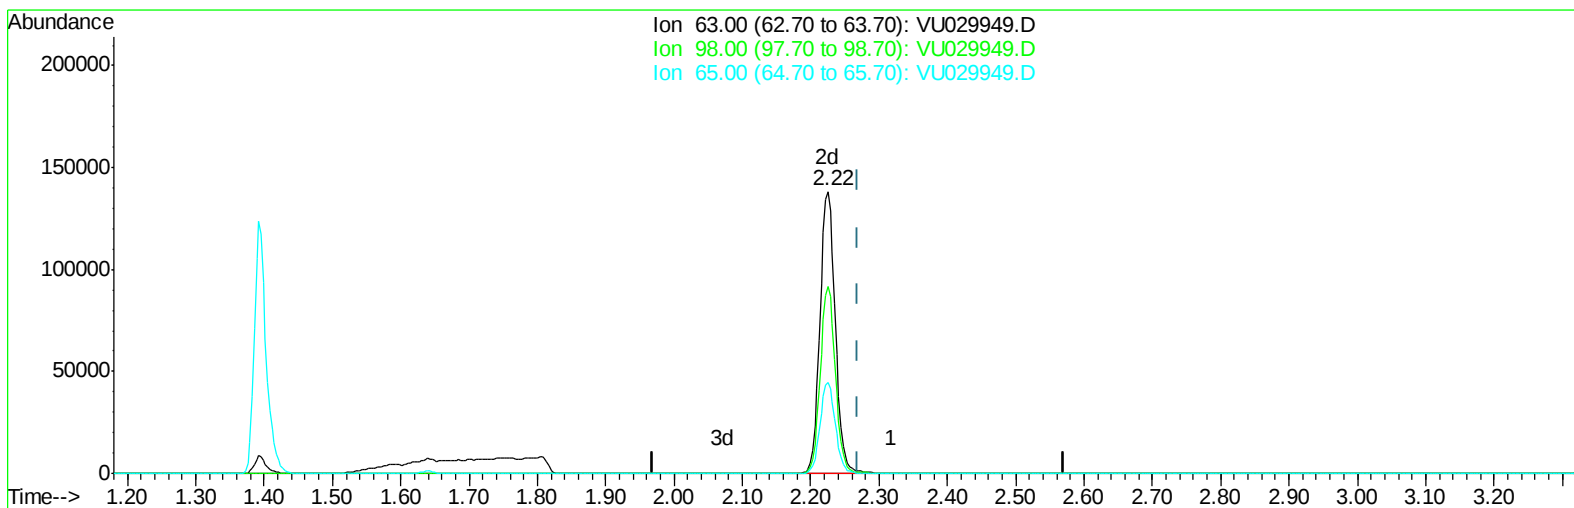

TIC: VU029949.D

(11) 1,1-Dichloroethene-d2 (S)

2.225min (-0.045) 31.91ug/L m

response 214803

Ion	Exp%	Act%
63.00	100	100
98.00	82.90	0.07#
65.00	23.60	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
 Data File : VU029949.D
 Acq On : 10 Mar 2019 15:15
 Operator : JC/SP
 Sample : K1818-12ME
 Misc : 5.80g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0R2ME

Manual Integrations
 APPROVED

MMDadoda
 3/11/2019 11:48:06 AM

Quant Time: Mar 11 08:00:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 11 07:10:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	585326	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	581859	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	292899	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	149110	41.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.50%
7) Chloroethane-d5	1.64	69	60554m	20.17	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	40.34%#
11) 1,1-Dichloroethene-d2	2.22	63	214803m	31.91	ug/L	-0.05
Spiked Amount	50.000	Range	60 - 125	Recovery	=	63.82%
21) 2-Butanone-d5	4.20	46	251184	90.78	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.78%
24) Chloroform-d	4.64	84	288074	41.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.90%
26) 1,2-Dichloroethane-d4	5.30	65	178199	43.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.52%
32) Benzene-d6	5.33	84	633189	43.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.34%
36) 1,2-Dichloropropane-d6	6.32	67	194137	44.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.66%
41) Toluene-d8	7.56	98	590515	42.44	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.88%
43) trans-1,3-Dichloropropene-	7.85	79	88105	41.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.14%
47) 2-Hexanone-d5	8.32	63	224778	95.39	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.39%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	317824	45.96	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.92%
64) 1,2-Dichlorobenzene-d4	11.86	152	250008	43.52	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.04%

Target Compounds					Qvalue
3) Chloromethane	1.32	50	53397	9.038 ug/L	97
6) Bromomethane	1.60	94	3258	2.685 ug/L	94
46) Tetrachloroethene	8.22	164	611195	169.412 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
Data File : VU029949.D
Acq On : 10 Mar 2019 15:15
Operator : JC/SP
Sample : K1818-12ME
Misc : 5.80g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0R2ME

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:48:06 AM

Quant Time: Mar 11 08:00:15 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 07:10:15 2019
Response via : Initial Calibration

