




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
Data File : VU029952.D
Acq On : 10 Mar 2019 16:25
Operator : JC/SP
Sample : K1818-16
Misc : 5.56g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0R6

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:48:24 AM

Quant Time: Mar 11 07:15:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 07:10:15 2019
Response via : Initial Calibration

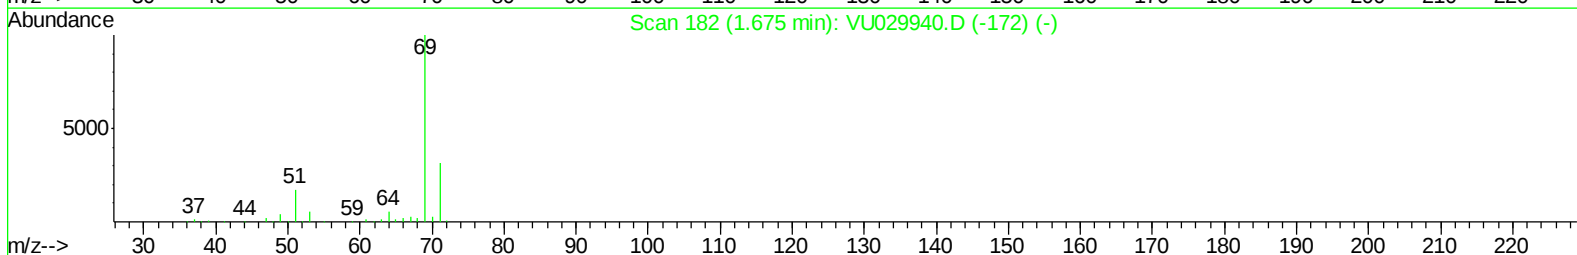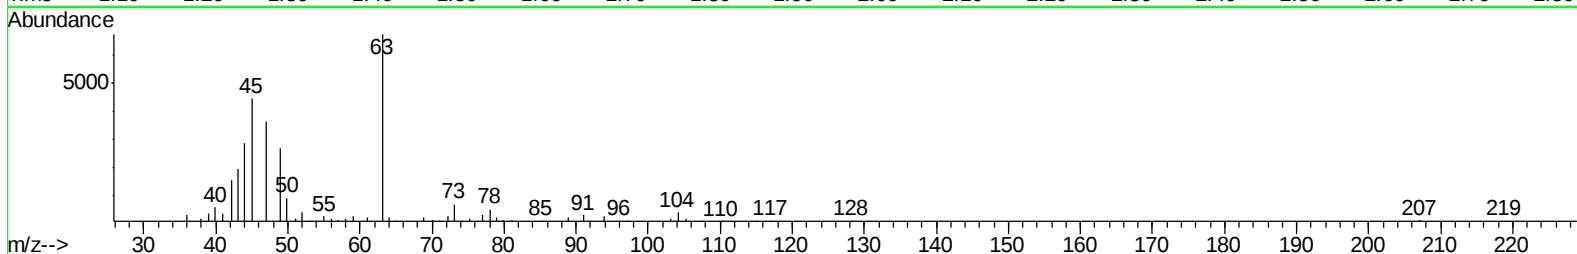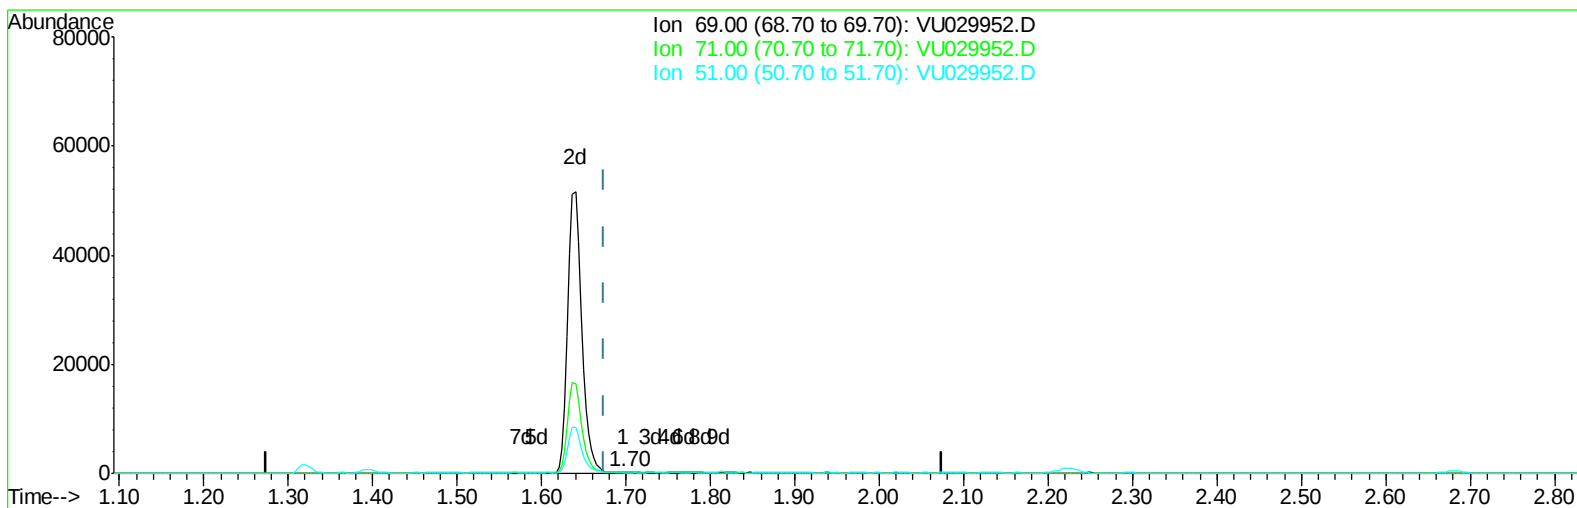

TIC: VU029952.D

(7) Chloroethane-d5 (S)

1.698min (+0.023) 0.12ug/L

response 378

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	38.62
51.00	24.10	5.03#
0.00	0.00	0.00




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
Data File : VU029952.D
Acq On : 10 Mar 2019 16:25
Operator : JC/SP
Sample : K1818-16
Misc : 5.56g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0R6

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:48:24 AM

Quant Time: Mar 11 07:15:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 07:10:15 2019
Response via : Initial Calibration

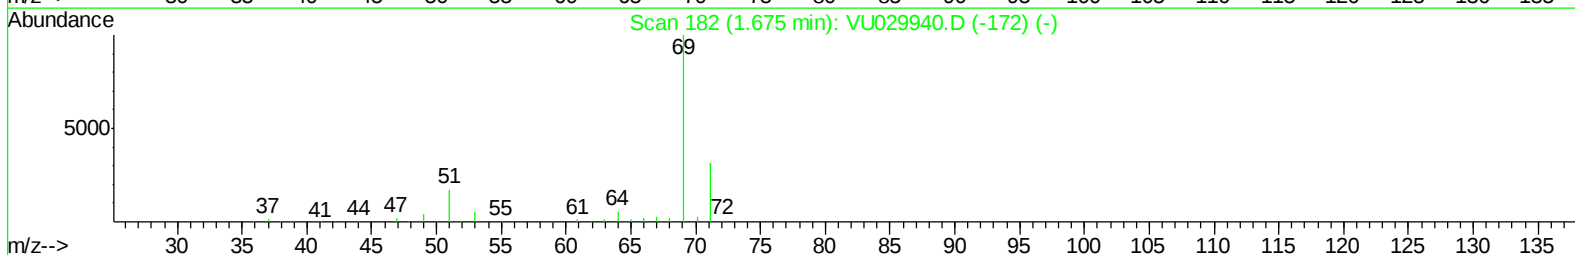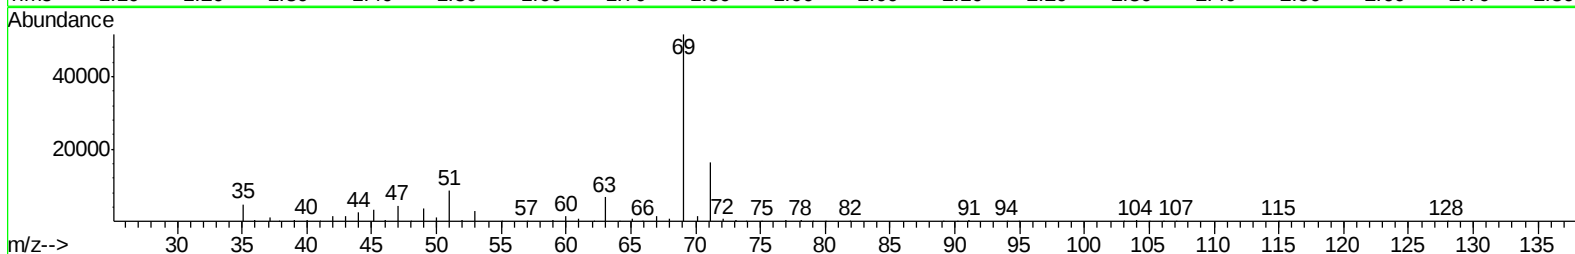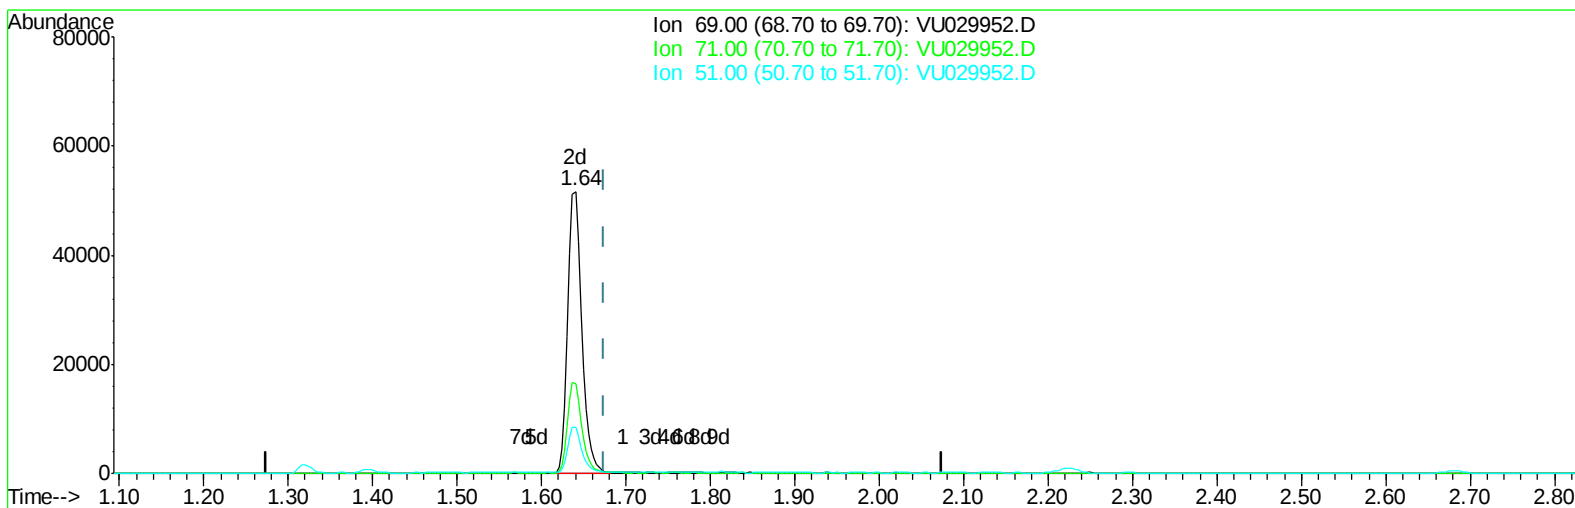

TIC: VU029952.D

(7) Chloroethane-d5 (S)

1.640min (-0.035) 19.22ug/L m

response 59341

Ion	Exp%	Act%
69.00	100	100
71.00	31.90	0.25#
51.00	24.10	0.03#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
 Data File : VU029952.D
 Acq On : 10 Mar 2019 16:25
 Operator : JC/SP
 Sample : K1818-16
 Misc : 5.56g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF0R6

Manual Integrations
 APPROVED

MMDadoda
 3/11/2019 11:48:24 AM

Quant Time: Mar 11 08:11:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Mar 11 07:10:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	602004	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	593750	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	297649	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	147607	40.19	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.38%
7) Chloroethane-d5	1.64	69	59341m	19.22	ug/L	-0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	38.44%#
11) 1,1-Dichloroethene-d2	2.23	63	216690	31.30	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.60%
21) 2-Butanone-d5	4.20	46	255515	89.79	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.79%
24) Chloroform-d	4.64	84	288745	40.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.78%
26) 1,2-Dichloroethane-d4	5.30	65	176870	42.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.46%
32) Benzene-d6	5.33	84	634353	42.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.74%
36) 1,2-Dichloropropane-d6	6.32	67	193653	43.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.66%
41) Toluene-d8	7.56	98	597103	42.06	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.12%
43) trans-1,3-Dichloropropene-	7.85	79	88886	41.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.20%
47) 2-Hexanone-d5	8.32	63	223440	92.92	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.92%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	318618	45.15	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.30%
64) 1,2-Dichlorobenzene-d4	11.86	152	251636	43.10	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.20%

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.32	50	52176	8.586	ug/L	99
6) Bromomethane	1.59	94	2939	2.355	ug/L	78
46) Tetrachloroethene	8.22	164	38144	10.361	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031219\
Data File : VU029952.D
Acq On : 10 Mar 2019 16:25
Operator : JC/SP
Sample : K1818-16
Misc : 5.56g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF0R6

Manual Integrations
APPROVED

MMDadoda
3/11/2019 11:48:24 AM

Quant Time: Mar 11 08:11:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Mar 11 07:10:15 2019
Response via : Initial Calibration

