


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031219\
 Data File : VU029939.D
 Acq On : 10 Mar 2019 11:16
 Operator : JC/SP
 Sample : BFB60
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB60

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031119WMA.M
 Title : VOC Analysis
 Last Update : Mon Mar 11 12:44:43 2019

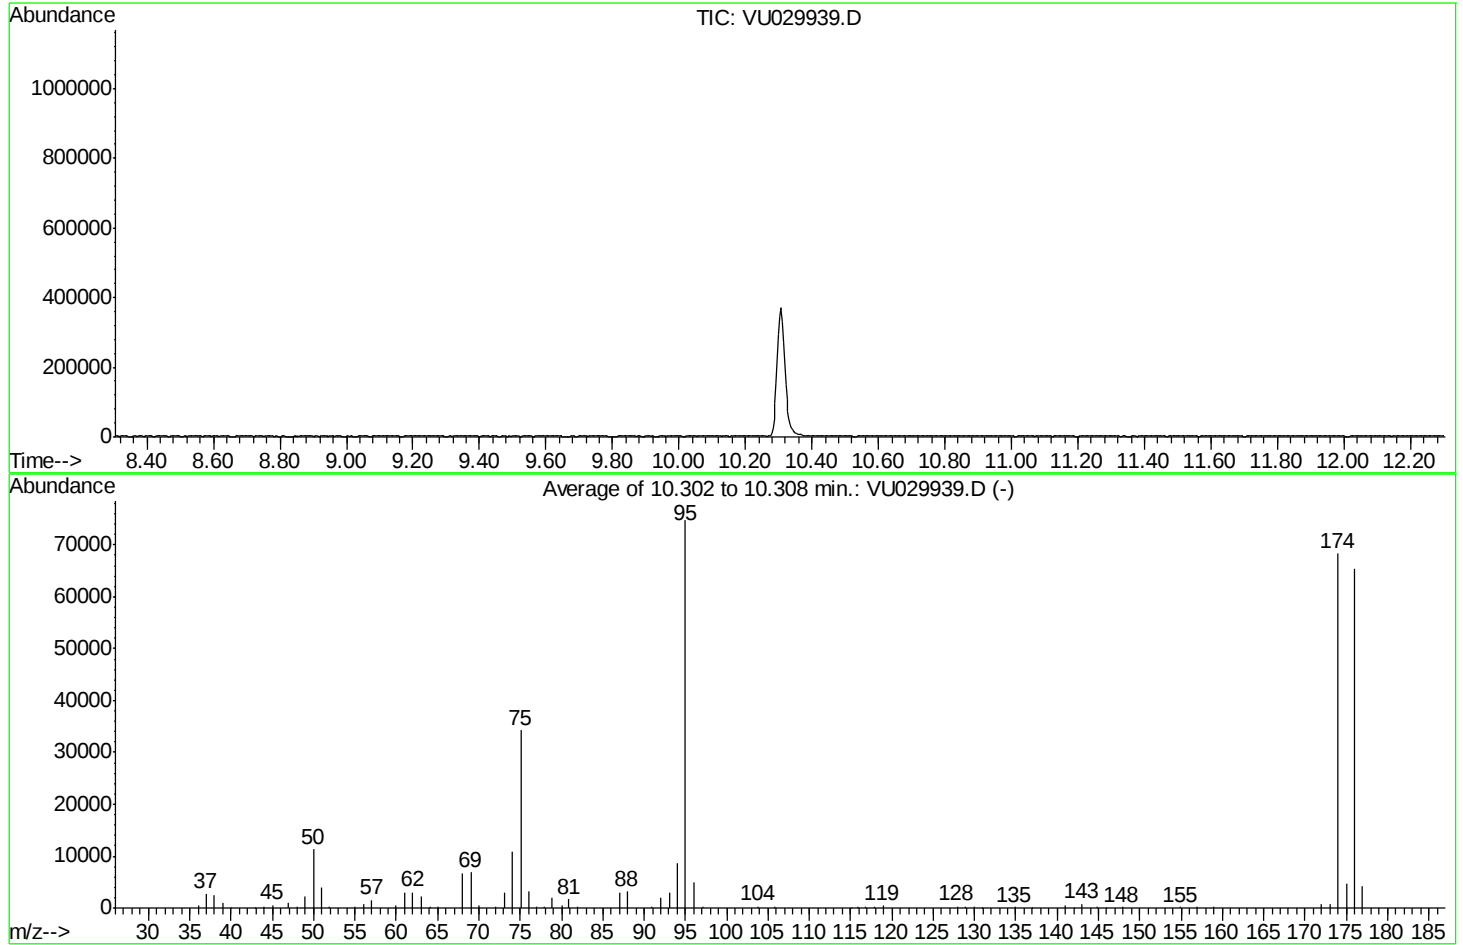

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	11293	PASS
75	95	30	80	45.8	34229	PASS
95	95	100	100	100.0	74744	PASS
96	95	5	9	6.8	5058	PASS
173	174	0.00	2	1.0	687	PASS
174	95	50	120	91.3	68272	PASS
175	174	5	9	6.9	4712	PASS
176	174	95	101	95.9	65477	PASS
177	176	5	9	6.4	4201	PASS

m/z	Abundance
40.00	1534.0
44.10	406.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	489.0
37.00	2825.0
38.00	2502.0
39.00	1031.0
40.00	1616.0
43.00	129.0
44.00	648.0
45.00	442.0
46.90	960.0
48.00	339.0
49.00	2379.0
50.00	11011.0
51.00	3731.0
51.90	169.0
55.00	278.0
56.00	916.0
57.00	1623.0
60.00	590.0
61.00	2871.0
62.00	3172.0
63.00	2392.0
64.10	264.0
65.00	303.0
68.00	6272.0
69.00	6650.0
70.00	473.0
72.00	334.0
73.10	2809.0
74.00	10795.0
75.00	33008.0
76.00	3449.0
76.90	243.0
77.80	331.0
78.90	1830.0
80.00	565.0
80.90	1565.0
82.00	384.0
87.00	2761.0
87.90	3007.0
90.90	231.0
92.00	2026.0
93.00	2947.0
94.00	8095.0
95.00	71712.0
96.00	5164.0
97.10	249.0
103.80	310.0
105.90	292.0
115.00	137.0
115.90	220.0
116.90	344.0
117.90	170.0
118.90	406.0
127.90	293.0
129.00	127.0
129.90	223.0
130.80	121.0
134.90	146.0
137.00	103.0
141.00	527.0
142.00	131.0
143.00	731.0
144.90	113.0
145.90	104.0
147.90	197.0
154.90	168.0
157.00	153.0
158.90	155.0
172.00	678.0
173.00	623.0
174.00	64336.0
175.00	4590.0
176.00	60744.0
177.00	4132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	521.0
37.00	2919.0
38.00	2500.0
39.00	985.0
40.00	1549.0
42.90	108.0
44.00	701.0
45.00	557.0
46.90	974.0
48.00	341.0
49.00	2419.0
50.00	11686.0
51.00	4038.0
51.90	157.0
55.00	304.0
56.00	878.0
57.00	1641.0
59.90	523.0
61.00	3060.0
62.00	3085.0
63.00	2282.0
64.10	302.0
65.00	381.0
68.00	6835.0
69.00	6949.0
70.00	573.0
72.00	379.0
73.00	2951.0
74.00	11246.0
75.00	35192.0
76.00	3340.0
76.90	301.0
77.90	369.0
78.90	1935.0
80.00	598.0
80.90	1767.0
82.00	353.0
87.00	3090.0
88.00	3246.0
90.80	325.0
92.00	2034.0
93.10	3166.0
94.00	8924.0
95.00	77128.0
96.00	5177.0
97.10	228.0
103.80	348.0
105.90	281.0
115.10	108.0
115.90	263.0
116.80	369.0
117.90	212.0
118.90	444.0
127.90	382.0
128.90	153.0
129.90	327.0
130.80	135.0
134.90	167.0
136.90	104.0
141.00	610.0
142.00	104.0
143.00	870.0
144.80	132.0
145.90	102.0
147.90	191.0
155.00	201.0
157.00	181.0
158.90	151.0
171.90	660.0
173.00	731.0
174.00	70024.0
175.00	4845.0
176.00	67584.0
177.00	4317.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60

m/z	Abundance
36.00	480.0
37.00	2619.0
38.00	2322.0
39.00	855.0
40.00	1512.0
44.00	761.0
45.00	581.0
46.90	750.0
48.00	370.0
49.00	2256.0
50.00	11184.0
51.00	3860.0
51.90	138.0
54.90	249.0
56.00	815.0
57.00	1570.0
59.90	497.0
61.00	2937.0
62.00	2778.0
63.00	2147.0
64.10	240.0
65.00	382.0
68.00	6629.0
69.00	6891.0
70.00	554.0
72.00	369.0
73.00	2908.0
74.00	10718.0
75.10	34488.0
76.00	3032.0
76.90	352.0
77.90	336.0
78.90	1839.0
80.00	507.0
80.90	1806.0
81.90	361.0
87.00	3362.0
88.00	3275.0
90.90	370.0
92.00	1832.0
93.00	3036.0
94.00	8819.0
95.00	75392.0
96.00	4834.0
97.00	188.0
103.80	347.0
105.80	237.0
115.90	301.0
116.80	381.0
117.80	253.0
119.00	392.0
127.90	350.0
128.90	156.0
129.90	346.0
130.90	117.0
134.90	183.0
136.90	102.0
140.90	616.0
143.00	863.0
144.90	163.0
145.90	112.0
147.90	168.0
155.00	243.0
157.00	214.0
158.90	106.0
171.90	612.0
173.00	708.0
174.00	70456.0
175.00	4703.0
176.00	68104.0
177.00	4156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB60