


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031221\
Data File : VU042562.D
Acq On : 11 Mar 2021 14:00
Operator : SY/MD
Sample : BFB24
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB24

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Mar 12 02:42:43 2021

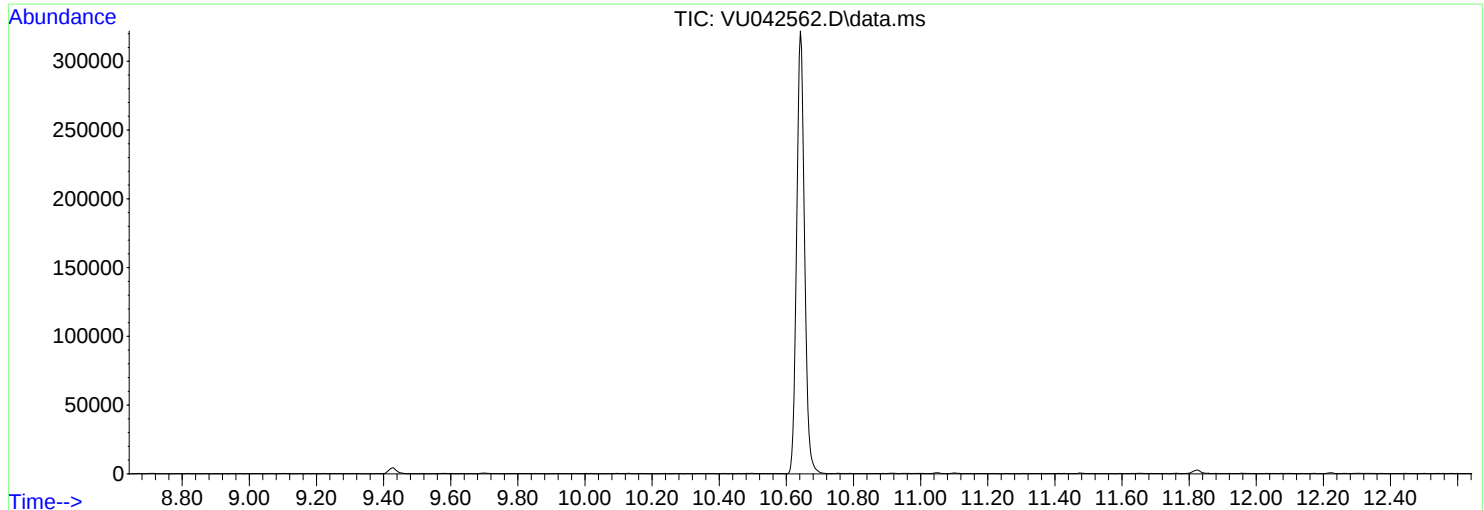

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	13321	PASS
75	95	30	80	56.8	31917	PASS
95	95	100	100	100.0	56171	PASS
96	95	5	9	7.1	4000	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	91.6	51427	PASS
175	174	5	9	8.6	4430	PASS
176	174	95	101	96.6	49653	PASS
177	176	5	9	6.9	3418	PASS

m/z	Abundance
35.90	676.0
37.00	4111.0
38.00	3620.0
39.00	1510.0
39.90	147.0
43.90	796.0
44.90	691.0
45.80	112.0
46.90	595.0
47.80	457.0
49.00	3181.0
50.00	12809.0
51.00	3906.0
51.90	180.0
54.90	242.0
55.90	1119.0
57.00	1998.0
57.90	132.0
59.90	637.0
61.00	3296.0
62.00	3332.0
63.00	2634.0
64.00	318.0
64.90	341.0
67.00	224.0
68.00	6489.0
69.00	6585.0
70.00	569.0
71.90	330.0
73.00	3399.0
74.00	11004.0
75.00	31192.0
76.00	2864.0
76.90	303.0
77.60	206.0
78.80	2757.0
79.90	673.0
80.90	2937.0
81.80	677.0
86.90	1944.0
87.90	2024.0
90.90	338.0
91.90	1985.0
93.00	2875.0
94.00	7479.0
95.00	55360.0
96.00	4122.0
103.80	381.0
104.80	123.0
105.80	338.0
110.80	119.0
115.80	297.0
116.90	503.0
117.90	250.0
118.80	457.0
127.80	240.0
129.80	343.0
134.70	110.0
140.80	833.0
142.80	849.0
144.80	143.0
147.90	203.0
154.80	204.0
156.80	142.0
170.90	112.0
171.90	660.0
173.90	49184.0
174.90	4435.0
175.90	47160.0
176.90	3395.0
177.80	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
35.90	693.0
37.00	4136.0
38.00	3511.0
39.00	1669.0
39.90	124.0
44.00	789.0
45.00	724.0
45.80	102.0
46.90	558.0
47.80	474.0
49.00	3397.0
50.00	13764.0
51.00	4372.0
52.00	191.0
54.90	209.0
55.90	1222.0
57.00	1964.0
57.90	111.0
59.90	589.0
61.00	3587.0
62.00	3540.0
63.00	2719.0
64.00	305.0
65.00	341.0
67.00	209.0
68.00	7104.0
69.00	6781.0
70.00	581.0
71.90	299.0
73.00	3461.0
74.00	11671.0
75.00	32736.0
76.00	3007.0
76.90	364.0
77.90	200.0
78.90	2794.0
79.90	719.0
80.90	3122.0
81.80	743.0
83.00	104.0
86.90	2038.0
87.90	1993.0
90.90	319.0
91.90	2114.0
93.00	2872.0
94.00	7893.0
95.00	58008.0
96.00	4165.0
103.80	419.0
104.80	127.0
105.80	412.0
110.90	106.0
115.90	330.0
116.90	581.0
117.80	306.0
118.80	457.0
127.80	270.0
129.80	367.0
131.00	124.0
140.90	852.0
141.80	102.0
142.90	928.0
144.80	170.0
147.80	210.0
154.90	197.0
156.80	117.0
170.40	102.0
170.90	118.0
171.90	742.0
173.90	53104.0
174.90	4588.0
175.90	51192.0
176.90	3559.0
177.80	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
35.90	664.0
37.00	3801.0
37.90	3228.0
39.00	1576.0
39.90	114.0
44.00	743.0
45.00	651.0
47.00	473.0
47.80	435.0
49.00	3242.0
50.00	13391.0
51.00	4379.0
52.00	203.0
54.90	177.0
55.90	1196.0
57.00	1762.0
59.90	567.0
61.00	3540.0
62.00	3446.0
63.00	2518.0
63.90	250.0
64.90	293.0
66.90	209.0
68.00	6825.0
69.00	6364.0
70.00	562.0
71.90	276.0
73.00	3146.0
74.00	11291.0
75.00	31824.0
76.00	2732.0
76.90	388.0
78.00	216.0
78.90	2680.0
79.90	732.0
80.90	2968.0
81.80	739.0
83.00	114.0
85.90	113.0
86.90	1859.0
87.90	1824.0
90.90	248.0
91.90	1939.0
93.00	2601.0
94.00	7593.0
95.00	55144.0
96.00	3714.0
103.80	426.0
104.80	101.0
105.90	435.0
115.90	320.0
116.90	545.0
117.80	303.0
118.80	400.0
127.80	238.0
129.80	325.0
130.90	130.0
136.80	121.0
140.90	837.0
141.70	134.0
142.90	866.0
144.80	165.0
147.70	184.0
154.90	146.0
156.80	104.0
170.90	102.0
171.90	706.0
173.90	51992.0
175.00	4266.0
175.90	50608.0
176.90	3300.0
177.80	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24

m/z	Abundance
43.80	150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB24