

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031221\
 Data File : VU042584.D
 Acq On : 11 Mar 2021 23:55
 Operator : SY/MD
 Sample : M1654-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B90

Quant Time: Mar 12 02:44:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Mar 12 02:42:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	77711	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	75612	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	34233	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	24449	4.72	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.40%
7) Chloroethane-d5	1.919	69	19966	5.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.80%
11) 1,1-Dichloroethene-d2	2.575	63	41425	3.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.80%
20) 2-Butanone-d5	4.649	46	81835	48.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.22%
24) Chloroform-d	5.073	84	50700	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
26) 1,2-Dichloroethane-d4	5.713	65	34152	5.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.40%
32) Benzene-d6	5.735	84	93237	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.60%
36) 1,2-Dichloropropane-d6	6.703	67	29817	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.906	98	88162	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
43) trans-1,3-Dichloroprop...	8.189	79	11652	4.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.40%
46) 2-Hexanone-d5	8.645	63	61821	46.21	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.42%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	26023	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.60%
64) 1,2-Dichlorobenzene-d4	12.201	152	33817	5.45	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	109.00%
Target Compounds					Qvalue	
13) Acetone	2.658	43	1600	1.22	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031221\
Data File : VU042584.D
Acq On : 11 Mar 2021 23:55
Operator : SY/MD
Sample : M1654-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B90

Quant Time: Mar 12 02:44:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Mar 12 02:42:43 2021
Response via : Initial Calibration

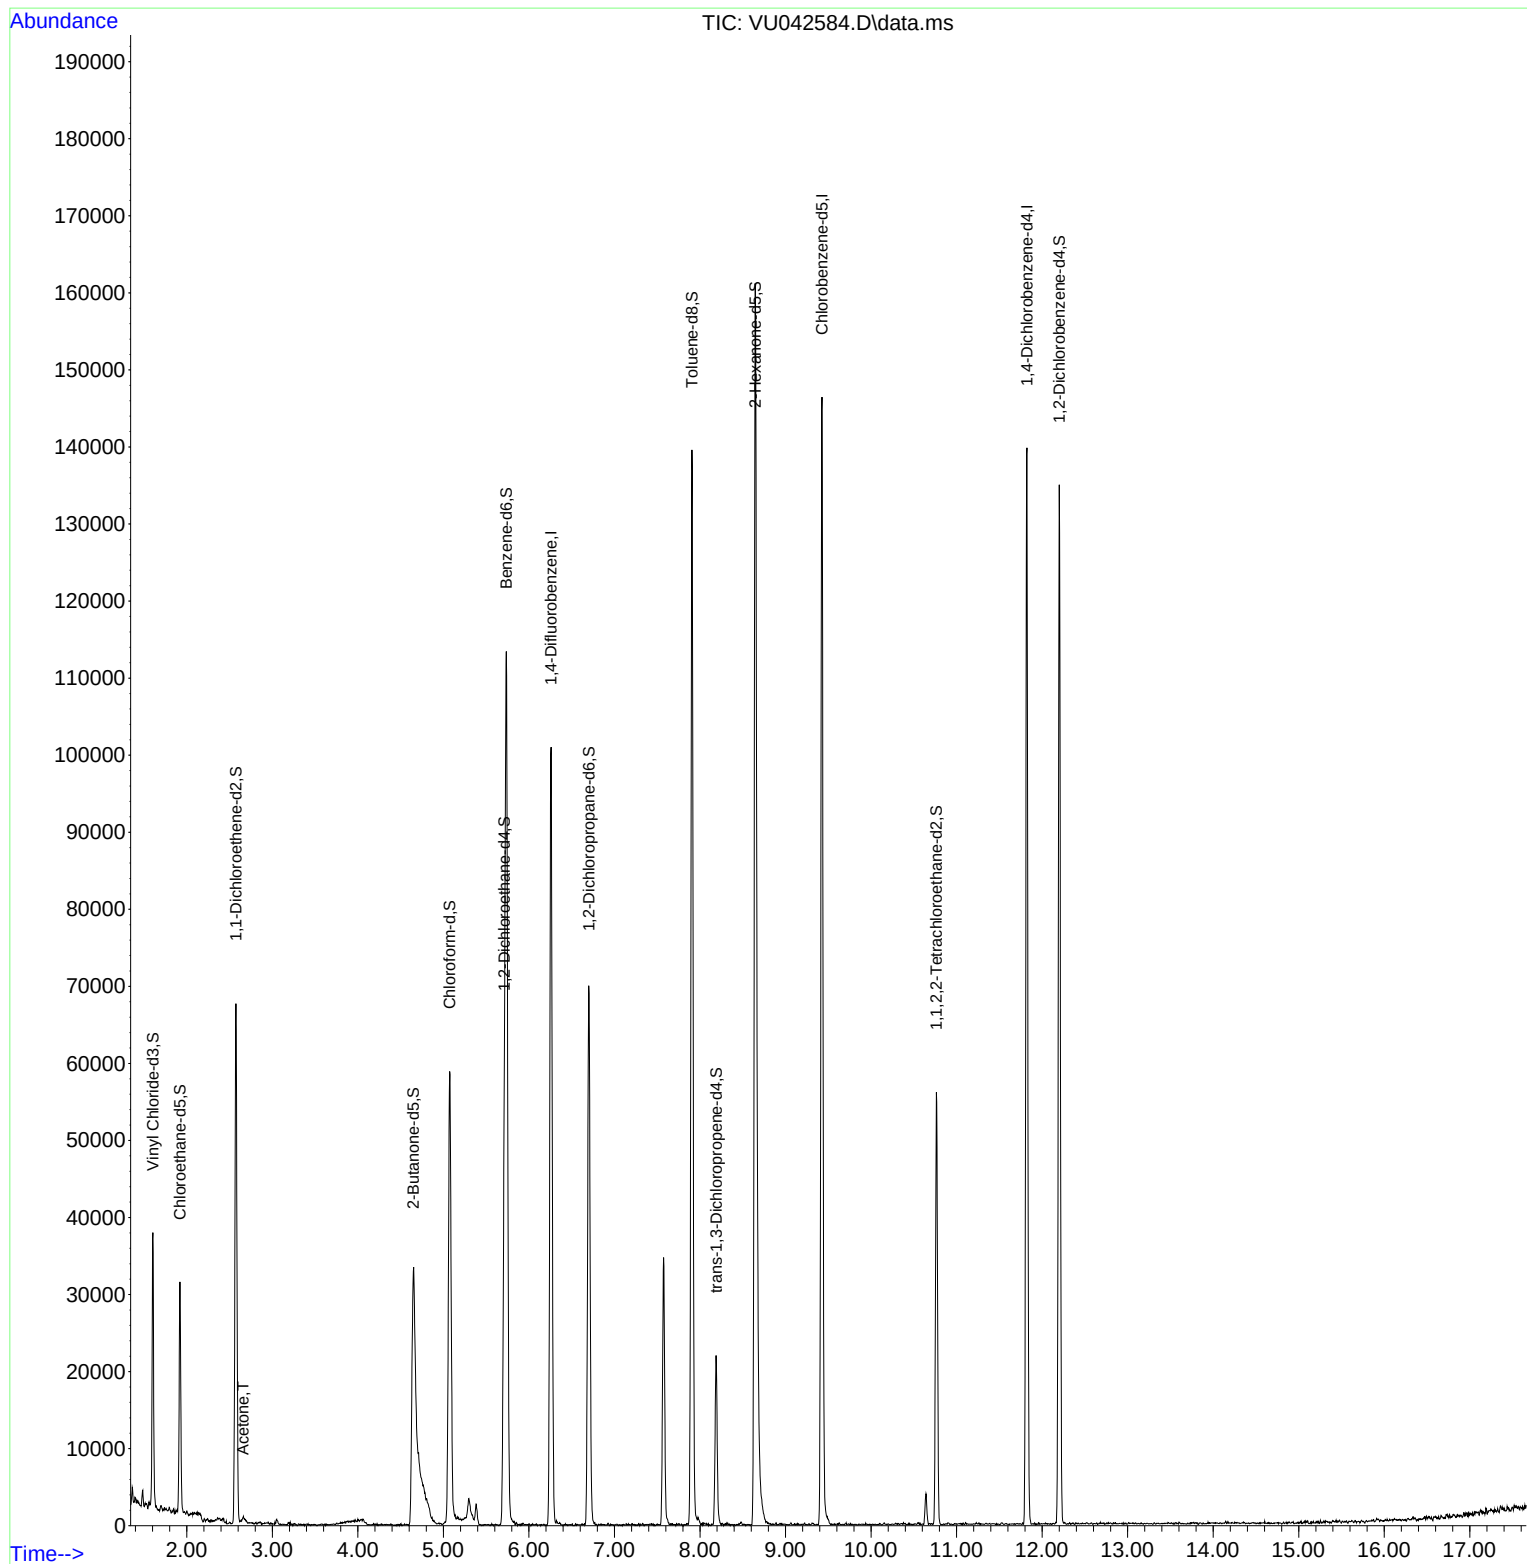

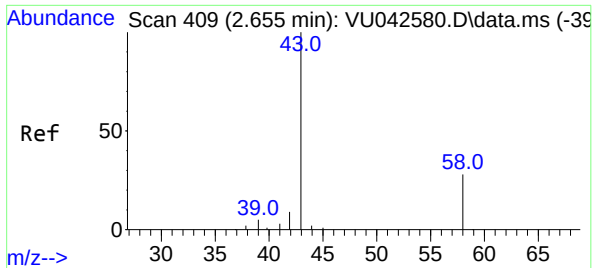

#13
 Acetone
 Concen: 1.22 ug/L
 RT: 2.658 min Scan# 410
 Delta R.T. 0.003 min
 Lab File: VU042584.D
 Acq: 11 Mar 2021 23:55

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B90

Tgt Ion:	43	Resp:	1600
Ion	Ratio	Lower	Upper
43	100		
58	21.3	0.0	55.8

