

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031221\
 Data File : VU042599.D
 Acq On : 12 Mar 2021 08:54
 Operator : SY/MD
 Sample : VU0312WBL03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK25

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rVB	34239	40245	13.03%	1.592%
2	1.919	172	180	192	rBV	28995	37496	12.14%	1.483%
3	2.575	369	384	401	rBV	65326	106308	34.43%	4.205%
4	4.652	1015	1030	1050	rBV2	28312	93567	30.30%	3.701%
5	5.073	1145	1161	1181	rBV	54584	119566	38.72%	4.729%
6	5.301	1221	1232	1244	rVB3	4696	9967	3.23%	0.394%
7	5.385	1248	1258	1269	rVB3	3034	6113	1.98%	0.242%
8	5.735	1345	1367	1384	rBV2	104910	282261	91.41%	11.165%
9	6.260	1516	1530	1553	rBV2	111226	210957	68.32%	8.344%
10	6.700	1653	1667	1684	rBV2	66173	129570	41.96%	5.125%
11	7.575	1927	1939	1959	rVB2	34004	60387	19.56%	2.389%
12	7.906	2030	2042	2063	rBV	142535	244982	79.34%	9.690%
13	8.189	2120	2130	2146	rBV2	20985	35529	11.51%	1.405%
14	8.649	2259	2273	2303	rBV	142486	308776	100.00%	12.214%
15	9.427	2502	2515	2535	rBV	167850	279489	90.52%	11.055%
16	10.642	2883	2893	2904	rBV3	11955	17781	5.76%	0.703%
17	10.767	2918	2932	2946	rBV2	51040	83898	27.17%	3.319%
18	11.822	3246	3260	3274	rBV	159758	255389	82.71%	10.102%
19	12.201	3367	3378	3391	rVB	128001	205833	66.66%	8.142%




Sum of corrected areas: 2528114

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031221\
Data File : VU042599.D
Acq On : 12 Mar 2021 08:54
Operator : SY/MD
Sample : VU0312WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

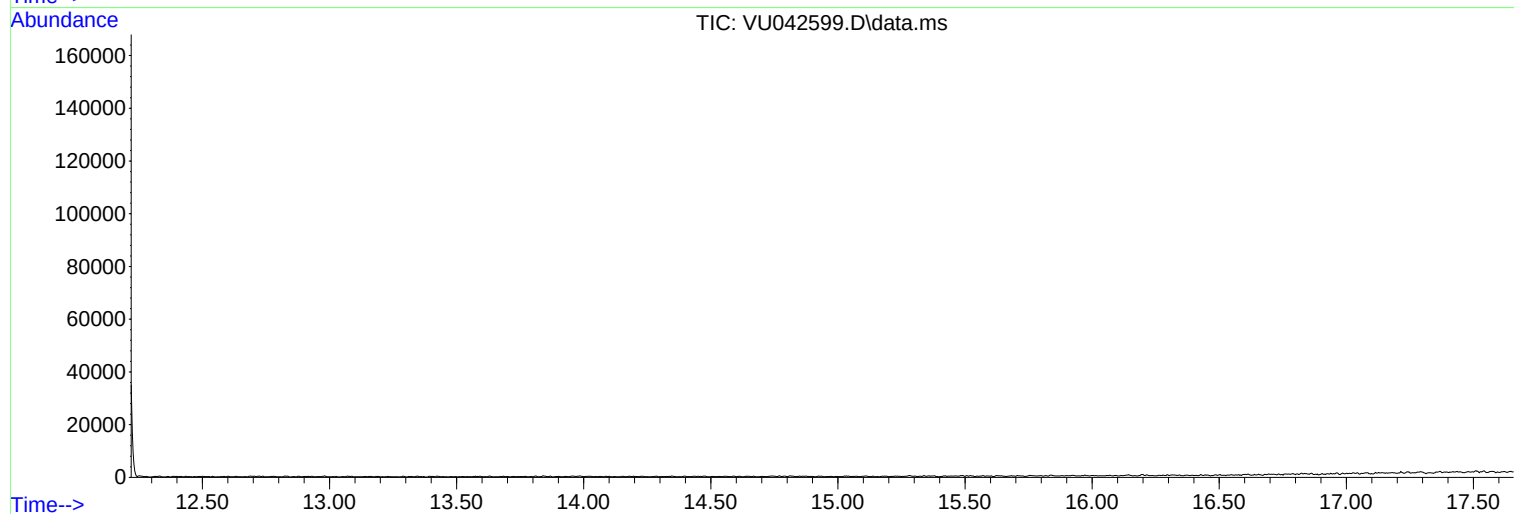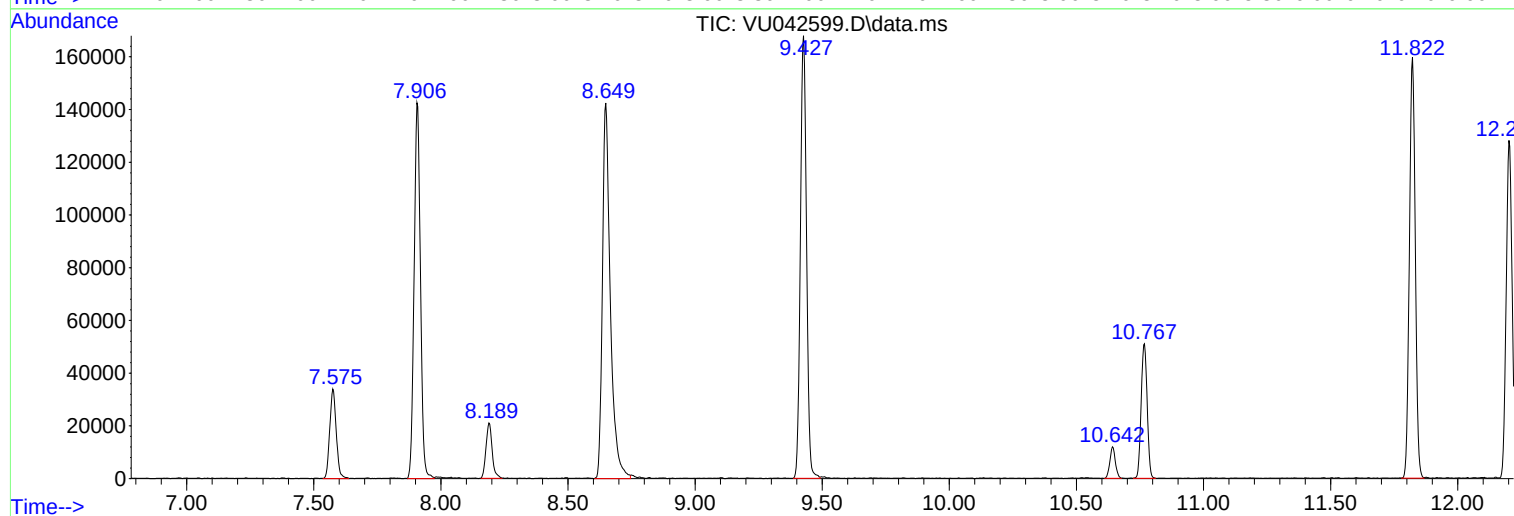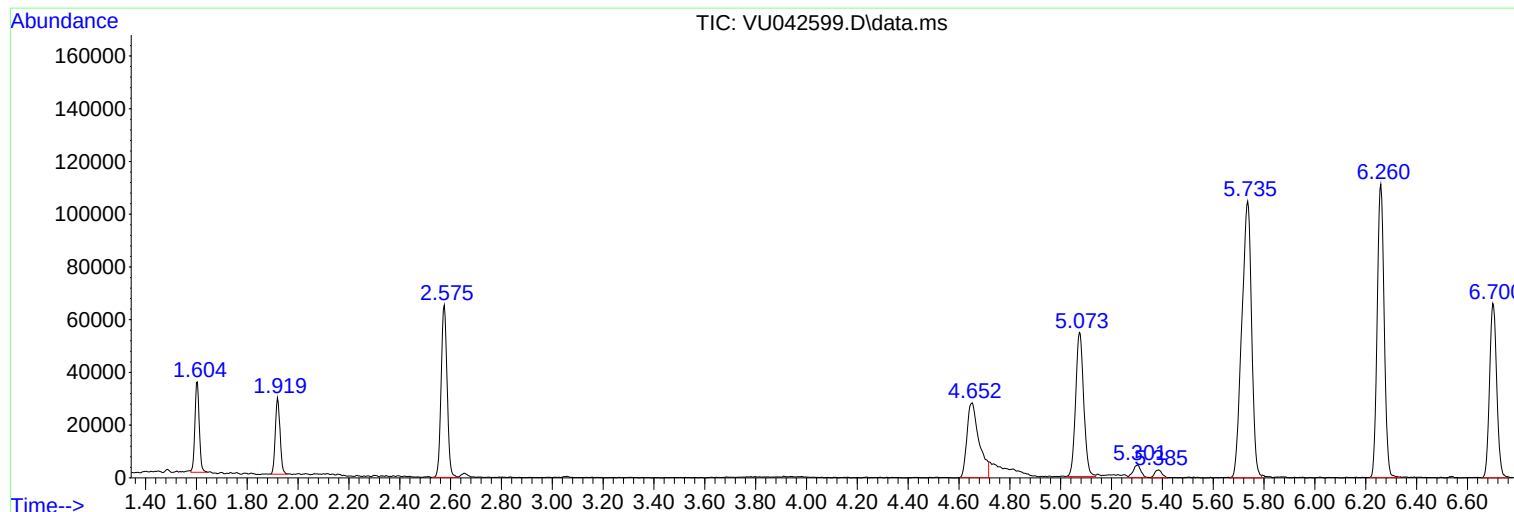

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031221\
Data File : VU042599.D
Acq On : 12 Mar 2021 08:54
Operator : SY/MD
Sample : VU0312WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031221\
Data File : VU042599.D
Acq On : 12 Mar 2021 08:54
Operator : SY/MD
Sample : VU0312WBL03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
