




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031224\
Data File : VU058062.D
Acq On : 12 Mar 2024 16:07
Operator : MD/SY
Sample : P1715-06DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGQN6DL

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 03/15/2024
Supervised By :Semsettin Yesilyurt 03/15/2024

Quant Time: Mar 13 02:02:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 13 01:58:39 2024
Response via : Initial Calibration

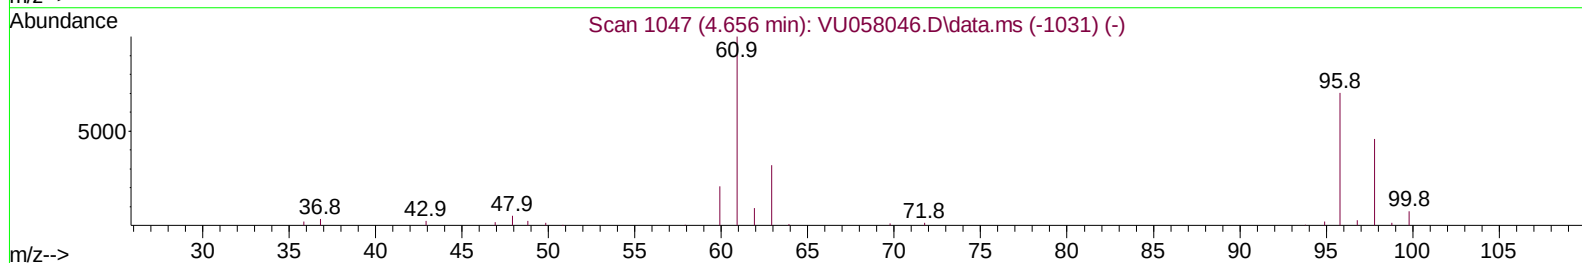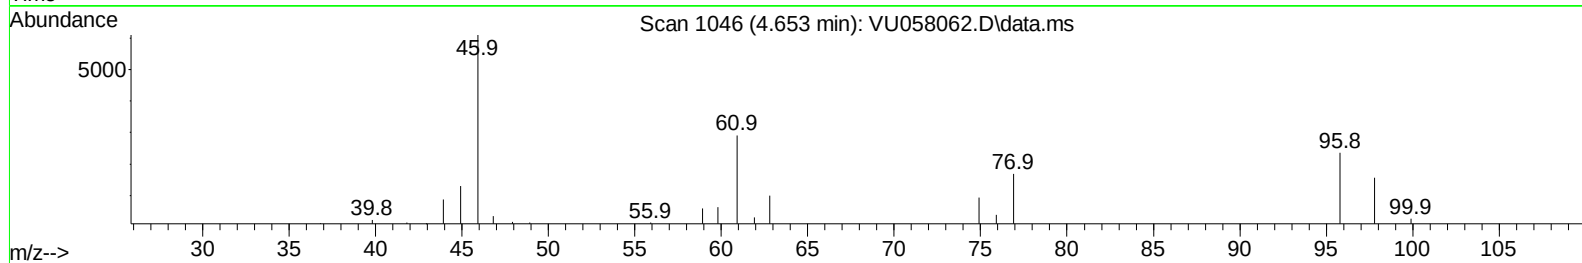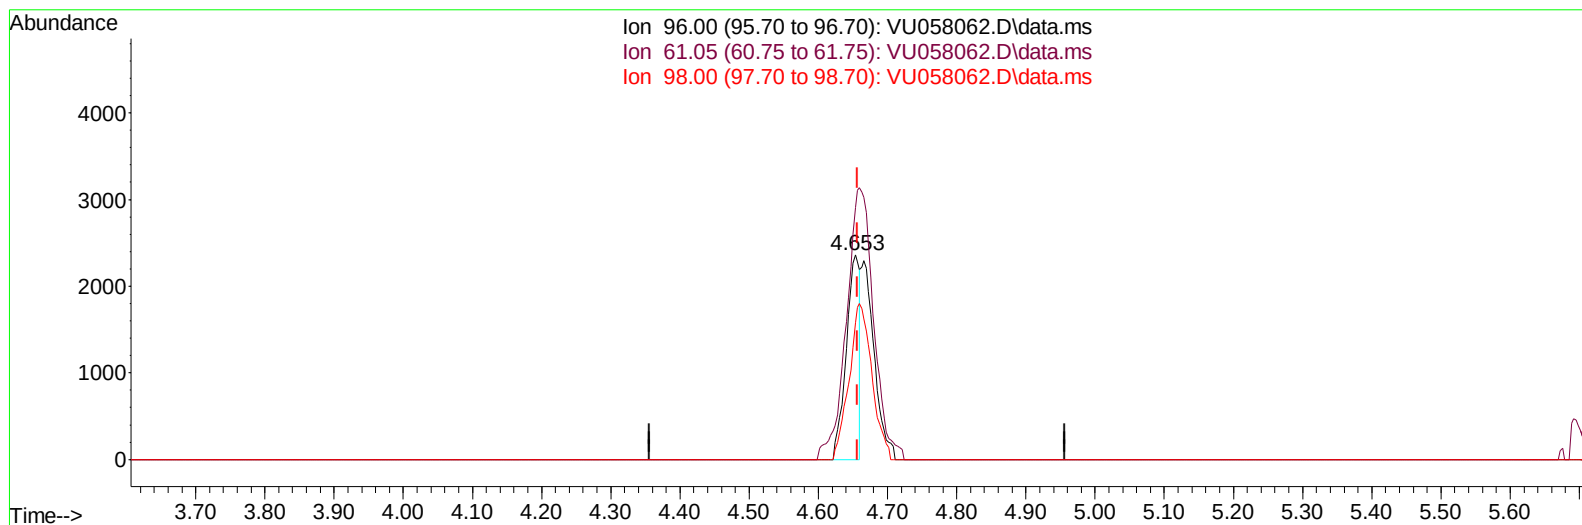

TIC: VU058062.D\data.ms

(22) cis-1,2-Dichloroethene (T)

4.653min (-0.003) 0.33 ug/L

response 3210

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	138.80	123.26
98.00	65.00	66.78
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031224\
Data File : VU058062.D
Acq On : 12 Mar 2024 16:07
Operator : MD/SY
Sample : P1715-06DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGQN6DL

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 03/15/2024
Supervised By :Semsettin Yesilyurt 03/15/2024

Quant Time: Mar 13 02:02:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 13 01:58:39 2024
Response via : Initial Calibration

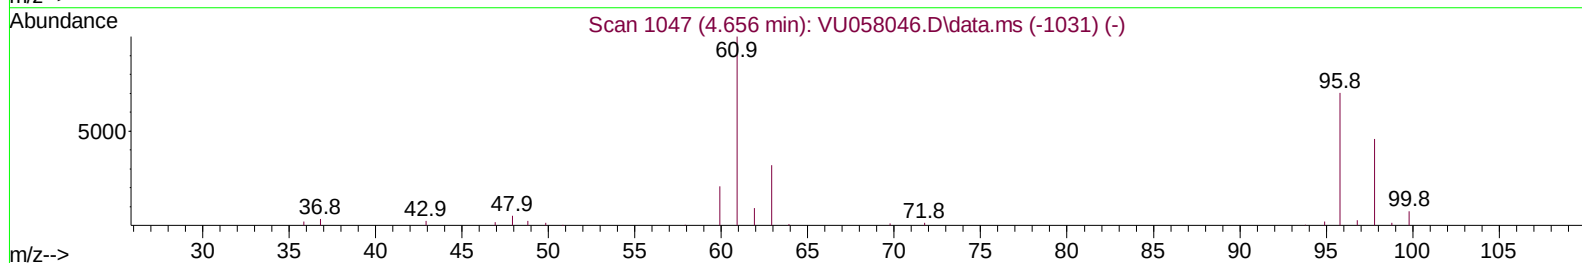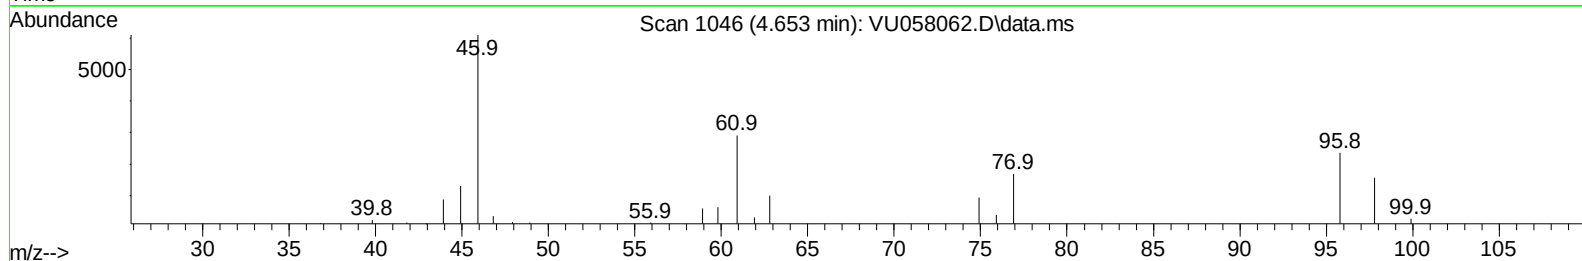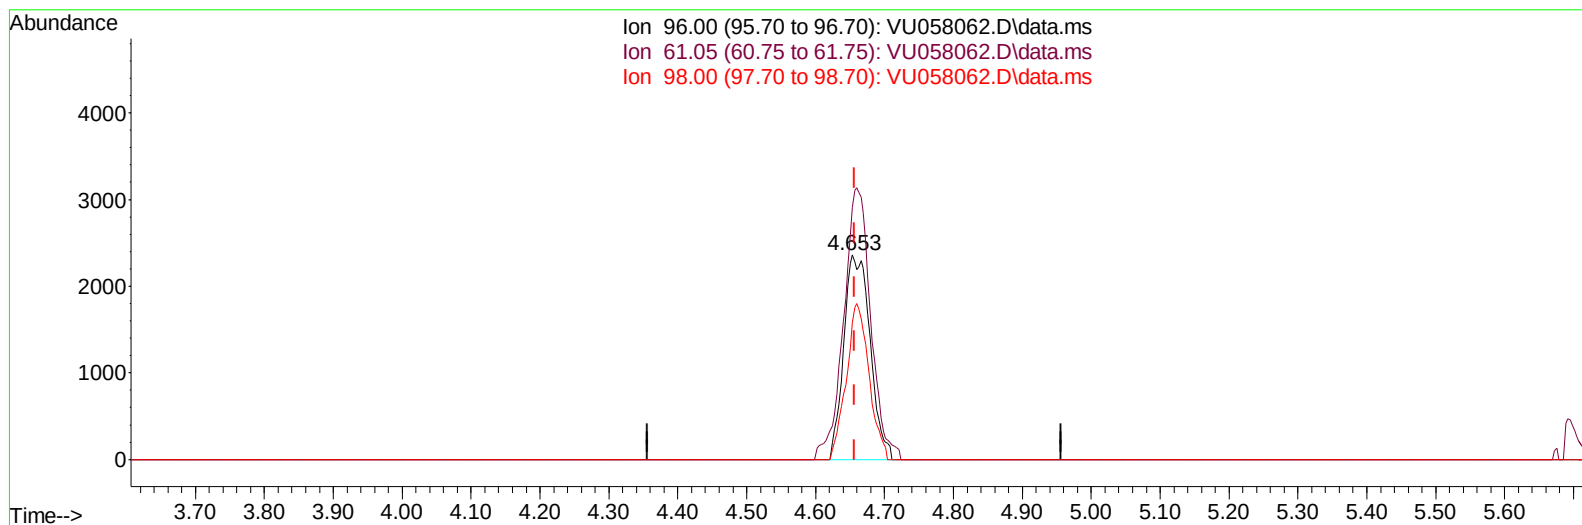

TIC: VU058062.D\data.ms

(22) cis-1,2-Dichloroethene (T)

4.653min (-0.003) 0.64 ug/L m

response 6249

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	138.80	123.26
98.00	65.00	66.78
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031224\
 Data File : VU058062.D
 Acq On : 12 Mar 2024 16:07
 Operator : MD/SY
 Sample : P1715-06DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGQN6DL

Manual IntegrationsAPPROVED

Quant Time: Mar 13 02:02:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 13 01:58:39 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/15/2024
 Supervised By :Semsettin Yesilyurt 03/15/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		135307	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		129178	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		58164	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.592	65		35495	3.646	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	73.000%	
7) Chloroethane-d5	1.904	69		34920	4.364	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	87.200%	
11) 1,1-Dichloroethene-d2	2.560	65		16466	3.909	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	78.200%	
20) 2-Butanone-d5	4.611	46		97257	60.633	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	121.260%	
24) Chloroform-d	5.052	84		88755	4.820	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	96.400%	
26) 1,2-Dichloroethane-d4	5.695	65		44492	5.333	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	106.600%	
32) Benzene-d6	5.717	84		172520	4.583	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	6.682	67		58121	5.079	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	101.600%	
41) Toluene-d8	7.891	98		142035	4.164	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	83.200%	
43) trans-1,3-Dichloroprop...	8.174	79		16441	4.178	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	83.600%	
46) 2-Hexanone-d5	8.624	63		80521	60.941	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	121.880%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		37891	5.399	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	108.000%	
66) 1,2-Dichlorobenzene-d4	12.190	152		48471	5.060	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	101.200%	
Target Compounds							
22) cis-1,2-Dichloroethene	4.653	96		6249m	0.639	ug/L	
34) Trichloroethene	6.541	95		8770	0.841	ug/L	99
47) Tetrachloroethene	8.547	164		19593	2.708	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031224\
Data File : VU058062.D
Acq On : 12 Mar 2024 16:07
Operator : MD/SY
Sample : P1715-06DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGQN6DL

Manual IntegrationsAPPROVED

Quant Time: Mar 13 02:02:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 13 01:58:39 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 03/15/2024
Supervised By :Semsettin Yesilyurt 03/15/2024

