


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031224\
Data File : VU058045.D
Acq On : 12 Mar 2024 08:28
Operator : MD/SY
Sample : BFB120
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB120

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Mar 14 04:37:22 2024

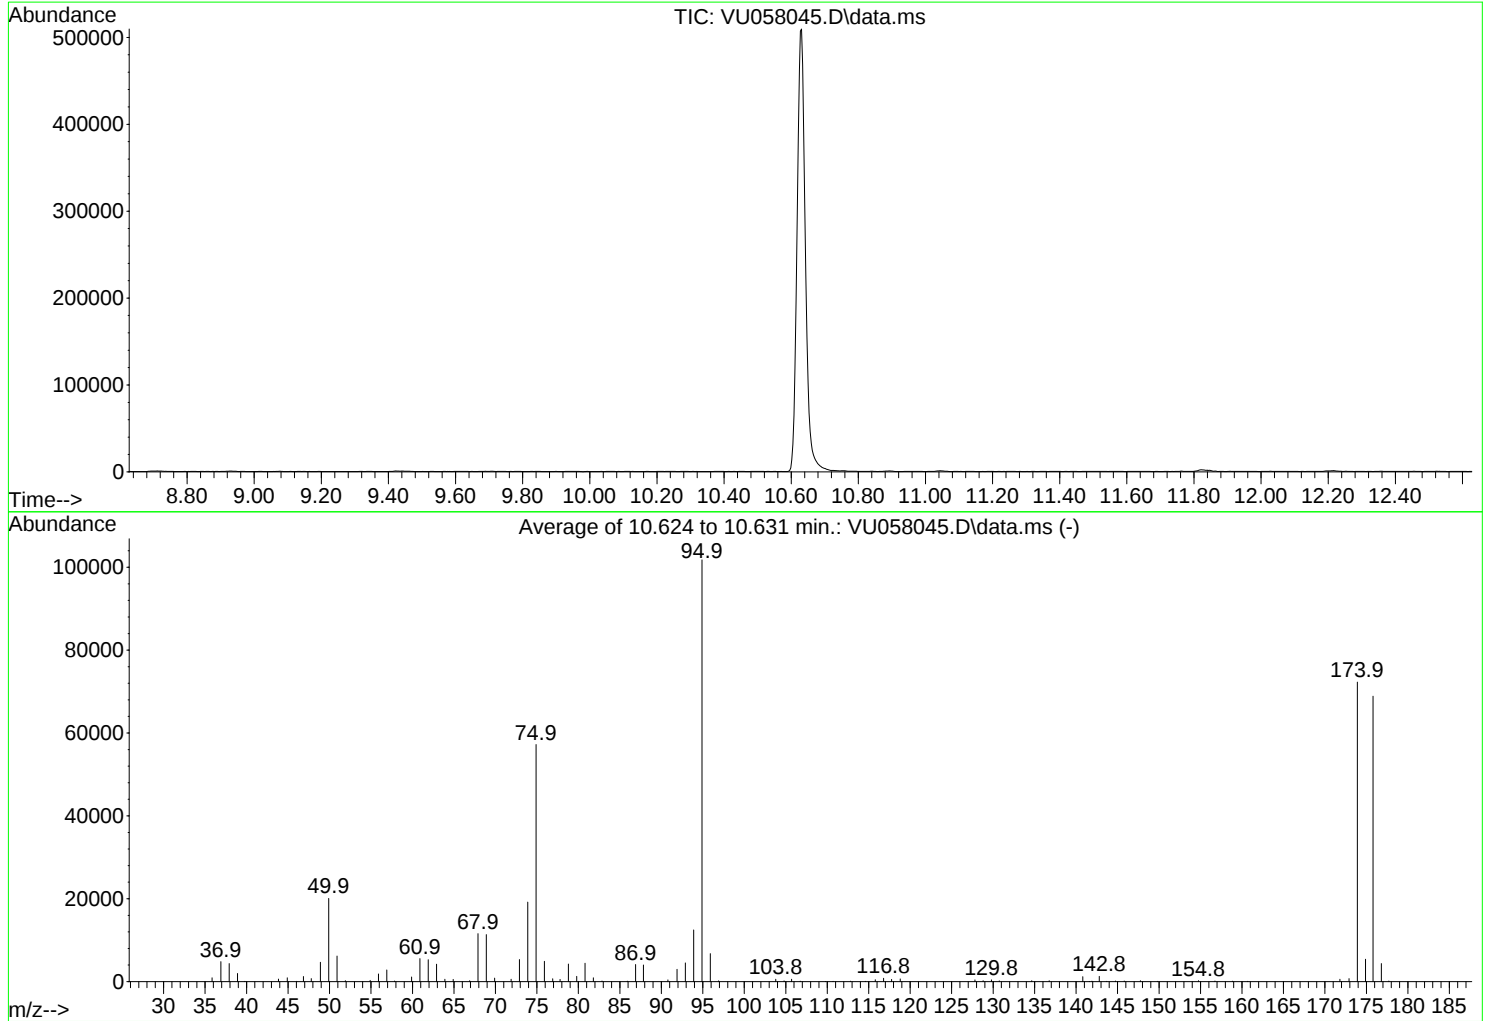

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	20093	PASS
75	95	30	80	56.2	57211	PASS
95	95	100	100	100.0	101787	PASS
96	95	5	9	6.6	6745	PASS
173	174	0.00	2	1.0	746	PASS
174	95	50	120	71.0	72301	PASS
175	174	5	9	7.5	5403	PASS
176	174	95	101	95.3	68885	PASS
177	176	5	9	6.4	4375	PASS

Scan 2890 (10.582 min): VU058045.D\data.ms
BFB120

m/z	Abundance
39.80	133.0
43.80	283.0

Instrument :
MSVOA_U
ClientSampleId :
BFB120

m/z	Abundance
35.80	871.0
36.90	4867.0
37.90	3988.0
38.90	1821.0
39.90	242.0
43.90	881.0
44.90	944.0
46.90	1189.0
47.80	798.0
48.90	4240.0
49.90	18920.0
50.90	5972.0
51.90	228.0
54.90	315.0
55.90	1805.0
56.90	2620.0
57.90	155.0
59.90	1073.0
60.90	5401.0
61.90	5038.0
62.90	3980.0
63.90	554.0
64.90	463.0
66.90	179.0
67.90	11229.0
68.90	10726.0
69.90	760.0
71.90	585.0
72.90	5096.0
73.90	17944.0
74.90	53840.0
75.90	4732.0
76.90	613.0
77.80	520.0
78.80	4193.0
79.80	1211.0
80.80	4293.0
81.80	882.0
82.80	155.0
85.90	171.0
86.90	3926.0
87.90	3853.0
90.80	410.0
91.90	2766.0
92.90	4255.0
93.90	11567.0
94.90	96208.0
95.90	6452.0
96.80	198.0
103.80	547.0
104.80	170.0
105.70	508.0
106.70	119.0
110.70	112.0
112.80	105.0
114.60	106.0
115.80	445.0
116.80	783.0
117.70	510.0
118.80	681.0
127.80	422.0
128.80	190.0
129.80	380.0
130.80	165.0
134.60	209.0
136.80	218.0
140.80	1010.0
141.60	134.0
142.80	1187.0
143.70	117.0
144.80	178.0
145.80	149.0
147.70	197.0
154.80	190.0
156.70	158.0
158.90	123.0
160.70	113.0
171.80	553.0
172.90	720.0
173.90	66488.0
174.90	5310.0
175.80	63064.0
176.80	4184.0
177.70	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB120

m/z	Abundance
35.80	931.0
36.90	4911.0
37.90	4499.0
38.90	1985.0
39.90	188.0
43.90	924.0
44.90	931.0
46.10	109.0
46.80	1247.0
47.80	782.0
48.90	4833.0
49.90	20688.0
50.90	6338.0
51.90	210.0
54.90	344.0
55.90	1945.0
56.90	2916.0
57.90	180.0
59.90	1153.0
60.90	5671.0
61.90	5467.0
62.90	4294.0
63.90	646.0
64.90	557.0
66.90	245.0
67.90	11873.0
68.90	11675.0
69.90	877.0
71.90	622.0
72.90	5490.0
73.90	19648.0
74.90	59008.0
75.90	5113.0
76.90	755.0
77.80	558.0
78.80	4360.0
79.80	1346.0
80.80	4523.0
81.80	959.0
82.90	161.0
85.90	144.0
86.90	4261.0
87.80	4055.0
90.80	439.0
91.90	3093.0
92.90	4660.0
93.90	12768.0
94.90	104696.0
95.90	6925.0
96.90	212.0
103.80	601.0
104.80	229.0
105.70	594.0
106.70	114.0
110.70	110.0
112.80	109.0
114.60	102.0
115.80	460.0
116.80	836.0
117.80	553.0
118.80	680.0
127.80	445.0
128.80	237.0
129.80	445.0
130.80	173.0
134.70	278.0
136.80	241.0
140.80	1218.0
141.90	172.0
142.80	1309.0
143.70	102.0
144.70	178.0
145.80	148.0
147.70	224.0
149.80	101.0
154.70	235.0
156.70	158.0
158.90	115.0
160.70	109.0
171.80	586.0
172.90	785.0
173.90	74256.0
174.90	5581.0
175.80	70864.0
176.80	4444.0
177.70	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB120

m/z	Abundance
35.90	939.0
36.90	4741.0
37.90	4613.0
38.90	2085.0
39.80	156.0
43.90	913.0
44.90	912.0
46.00	127.0
46.80	1260.0
47.80	665.0
48.90	4932.0
49.90	20672.0
50.90	6227.0
51.90	218.0
54.90	331.0
55.90	1840.0
56.90	2963.0
57.80	147.0
59.90	1103.0
60.90	5631.0
61.90	5388.0
62.90	4349.0
63.90	582.0
64.90	593.0
66.90	327.0
67.90	11614.0
68.90	11701.0
69.90	927.0
71.90	587.0
72.90	5382.0
73.90	19960.0
74.90	58784.0
75.90	4901.0
76.90	736.0
77.80	546.0
78.80	4218.0
79.80	1329.0
80.80	4467.0
81.80	998.0
82.90	139.0
86.90	4199.0
87.80	4107.0
90.80	458.0
91.90	3088.0
92.90	4641.0
93.90	13138.0
94.90	104456.0
95.90	6858.0
97.00	200.0
103.80	601.0
104.80	239.0
105.70	635.0
106.80	109.0
109.80	108.0
112.80	107.0
115.80	484.0
116.80	792.0
117.80	522.0
118.80	672.0
127.80	427.0
128.80	251.0
129.80	480.0
130.70	206.0
134.70	264.0
136.70	244.0
140.80	1314.0
141.90	204.0
142.80	1384.0
144.80	162.0
145.80	155.0
147.80	266.0
149.80	100.0
154.70	265.0
156.80	148.0
158.80	108.0
171.80	642.0
172.90	734.0
173.90	76160.0
174.90	5317.0
175.80	72728.0
176.80	4497.0
177.70	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB120