


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031319\
Data File : VU029972.D
Acq On : 11 Mar 2019 16:18
Operator : JC/SP
Sample : BFB31
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB31

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Title : VOC Analysis
Last Update : Thu Mar 14 01:36:14 2019

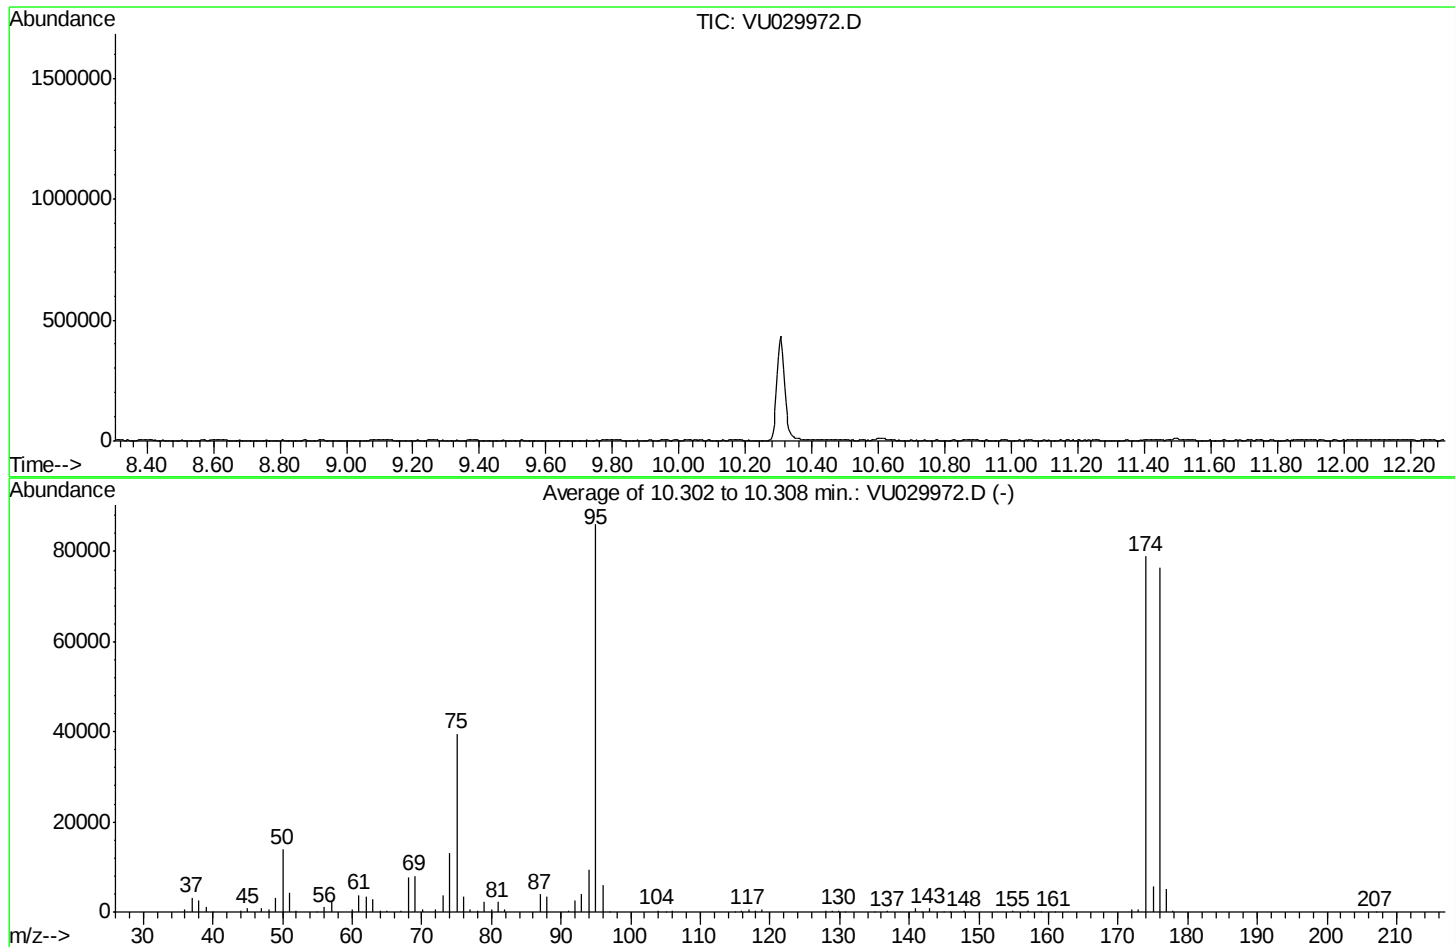

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	13802	PASS
75	95	30	80	46.0	39584	PASS
95	95	100	100	100.0	86042	PASS
96	95	5	9	6.8	5883	PASS
173	174	0.00	2	0.8	670	PASS
174	95	50	120	91.7	78909	PASS
175	174	5	9	7.1	5571	PASS
176	174	95	101	96.9	76488	PASS
177	176	5	9	6.6	5085	PASS

m/z	Abundance
40.00	2111.0
44.00	483.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	581.0
37.00	3245.0
38.00	2374.0
39.00	1234.0
40.00	2049.0
44.00	708.0
45.00	709.0
47.00	992.0
48.10	447.0
49.00	2894.0
50.00	13304.0
51.00	3917.0
52.00	264.0
54.80	131.0
56.00	1004.0
57.00	2190.0
60.00	681.0
61.00	3784.0
62.00	3413.0
63.00	2839.0
64.00	345.0
65.00	337.0
66.90	218.0
68.00	7493.0
69.00	7967.0
70.00	610.0
71.90	409.0
73.00	3679.0
74.00	13270.0
75.00	39264.0
76.00	3566.0
76.90	634.0
78.10	228.0
78.90	2124.0
80.00	574.0
80.90	2354.0
81.90	454.0
87.00	3895.0
88.00	3217.0
91.00	288.0
92.00	2259.0
93.00	4057.0
94.00	9138.0
95.00	84728.0
96.00	5884.0
97.00	112.0
103.90	360.0
105.10	142.0
105.90	332.0
115.90	333.0
116.90	457.0
117.90	372.0
119.00	464.0
127.90	268.0
128.90	184.0
129.80	296.0
135.00	131.0
137.10	117.0
140.90	759.0
141.80	100.0
142.90	780.0
144.90	107.0
145.90	182.0
147.90	228.0
154.80	172.0
157.00	213.0
158.90	102.0
160.90	113.0
171.90	641.0
173.00	653.0
174.00	74800.0
175.00	5340.0
176.00	72592.0
177.00	4966.0
177.90	126.0
207.00	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	525.0
37.00	3302.0
38.00	2531.0
39.00	1213.0
40.00	2082.0
44.00	621.0
45.00	775.0
47.00	1024.0
48.10	527.0
49.00	3220.0
50.00	14326.0
51.00	4373.0
52.00	272.0
54.80	135.0
56.00	1092.0
57.00	2413.0
60.00	712.0
61.00	3949.0
62.00	3439.0
63.00	2877.0
64.00	324.0
65.00	297.0
67.00	240.0
68.00	7999.0
69.00	8344.0
70.10	656.0
71.90	462.0
73.00	3753.0
74.00	13702.0
75.00	40880.0
76.00	3595.0
76.90	592.0
78.00	250.0
78.90	2272.0
80.00	643.0
80.90	2360.0
81.90	479.0
87.00	4111.0
88.00	3481.0
91.00	306.0
92.00	2552.0
93.00	4138.0
94.00	9574.0
95.00	88896.0
96.00	6156.0
97.00	128.0
103.90	387.0
105.00	122.0
105.90	349.0
115.00	103.0
115.90	285.0
116.90	539.0
117.90	354.0
118.90	486.0
127.90	259.0
128.90	235.0
129.90	307.0
130.70	103.0
134.90	133.0
136.90	153.0
140.90	849.0
142.90	879.0
144.90	104.0
145.90	147.0
147.90	268.0
154.90	222.0
157.00	147.0
160.90	114.0
171.90	665.0
172.90	697.0
174.00	81112.0
175.00	5723.0
176.00	78784.0
177.00	5215.0
177.90	177.0
207.00	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	461.0
37.00	3027.0
38.00	2472.0
39.00	1094.0
39.90	2216.0
44.00	597.0
45.00	704.0
47.00	877.0
48.10	465.0
49.00	3147.0
50.00	13778.0
51.00	4223.0
51.90	258.0
54.80	116.0
56.00	1027.0
57.00	2291.0
60.00	610.0
61.00	3649.0
62.00	3362.0
63.00	2741.0
64.00	283.0
65.00	266.0
66.90	221.0
67.10	218.0
68.00	7798.0
69.00	7686.0
70.10	574.0
71.90	453.0
73.00	3397.0
74.00	12623.0
75.00	38608.0
76.00	3300.0
76.90	513.0
77.90	316.0
78.90	2175.0
80.00	575.0
80.90	2073.0
81.90	401.0
87.00	3841.0
88.00	3357.0
91.00	313.0
92.00	2588.0
93.00	3754.0
94.10	9179.0
95.00	84504.0
96.00	5609.0
97.00	115.0
103.80	376.0
105.90	315.0
114.90	134.0
115.90	231.0
116.90	527.0
117.90	279.0
118.80	437.0
128.00	303.0
128.90	222.0
130.00	283.0
130.70	125.0
134.90	155.0
136.80	187.0
140.90	834.0
142.90	869.0
145.90	112.0
147.90	297.0
155.00	255.0
156.90	110.0
171.90	616.0
172.90	662.0
174.00	80816.0
175.00	5652.0
176.00	78088.0
177.00	5076.0
177.90	215.0
207.00	150.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31