

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031320\
 Data File : VU037248.D
 Acq On : 13 Mar 2020 17:46
 Operator : JC/MD
 Sample : L1900-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CONB8

Quant Time: Mar 14 01:14:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 14 00:24:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	123500	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	122384	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	52315	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	36295	4.48	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.60%
7) Chloroethane-d5	1.93	69	31085	5.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.60%
11) 1,1-Dichloroethene-d2	2.59	63	52645	3.15	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.00%
20) 2-Butanone-d5	4.67	46	101474	48.92	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.84%
24) Chloroform-d	5.10	84	69904	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.20%
26) 1,2-Dichloroethane-d4	5.74	65	46006	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.60%
32) Benzene-d6	5.76	84	137762	4.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.60%
36) 1,2-Dichloropropane-d6	6.73	67	44965	4.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.40%
41) Toluene-d8	7.92	98	124921	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
43) trans-1,3-Dichloropropene-	8.20	79	18113	4.61	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.20%
46) 2-Hexanone-d5	8.66	63	79798	48.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.60%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	35994	4.50	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.00%
64) 1,2-Dichlorobenzene-d4	12.21	152	46137	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Ovalue
13) Acetone	2.66	43	1920	1.130 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031320\
Data File : VU037248.D
Acq On : 13 Mar 2020 17:46
Operator : JC/MD
Sample : L1900-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONB8

Quant Time: Mar 14 01:14:07 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 14 00:24:25 2020
Response via : Initial Calibration

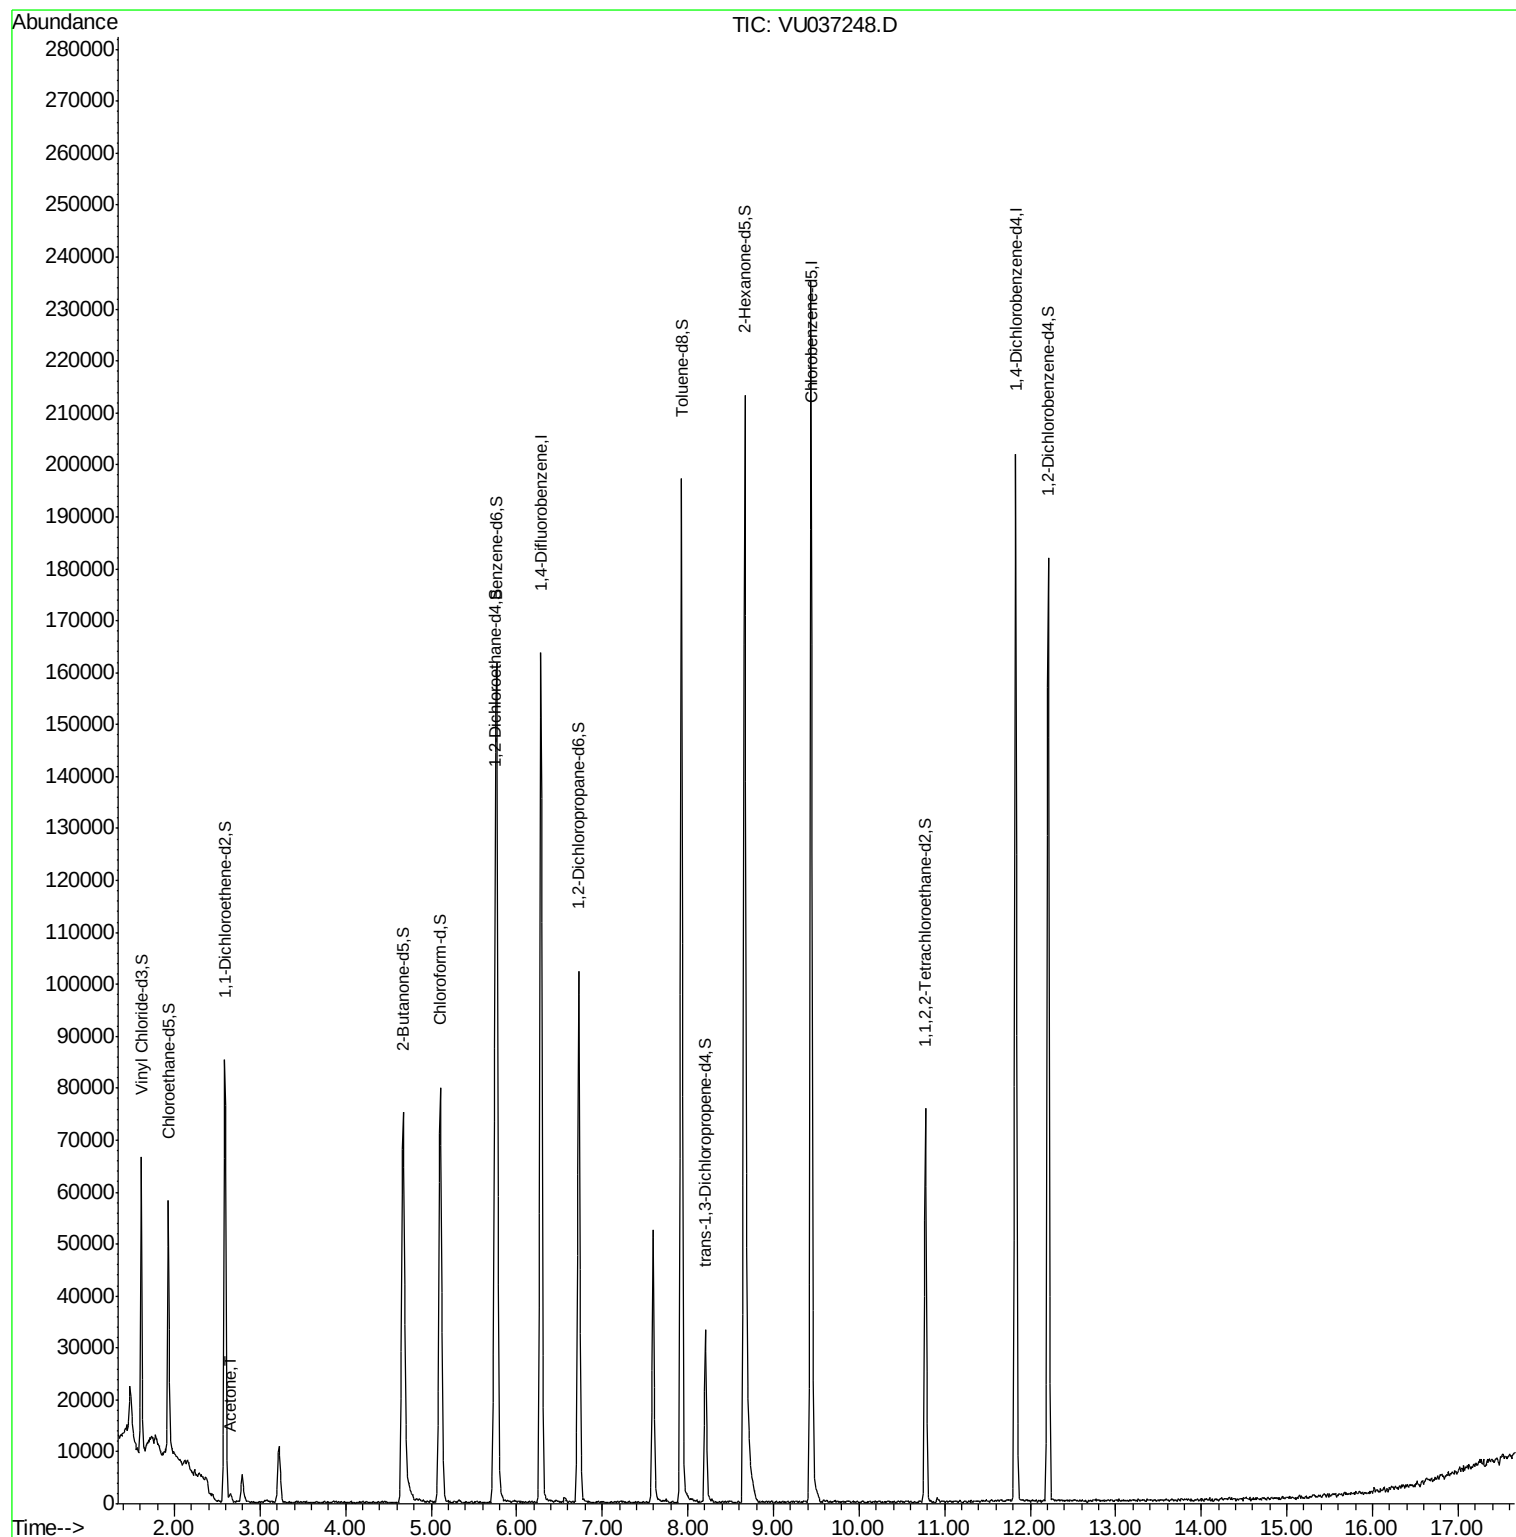

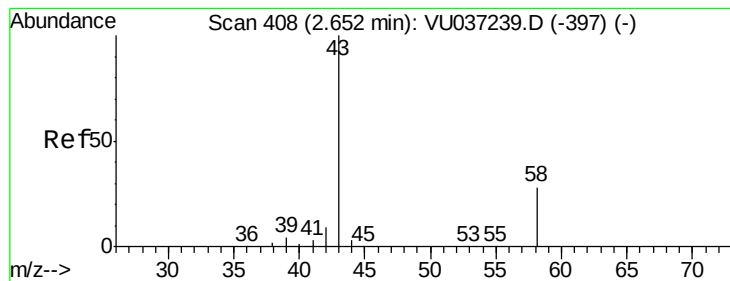

#13

Acetone

Concen: 1.130 ug/L

RT: 2.66 min Scan# 411

Delta R.T. 0.01 min

Lab File: VU037248.D

Acq: 13 Mar 2020 17:46

Instrument :
MSVOA_U
ClientSampleId :
CONB8

Tot Ion: 43 Resp: 1920

Ion Ratio Lower Upper

43 100

58 24.7 0.0 52.2

