

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031320\
 Data File : VU037249.D
 Acq On : 13 Mar 2020 18:11
 Operator : JC/MD
 Sample : L1900-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CONB9

Quant Time: Mar 14 01:28:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 14 00:24:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	122621	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	120915	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	51474	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	38519	4.78	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.60%
7) Chloroethane-d5	1.93	69	32711	5.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.00%
11) 1,1-Dichloroethene-d2	2.59	63	53944	3.25	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.00%
20) 2-Butanone-d5	4.67	46	100476	48.78	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.56%
24) Chloroform-d	5.11	84	72616	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
26) 1,2-Dichloroethane-d4	5.74	65	46586	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
32) Benzene-d6	5.76	84	139264	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
36) 1,2-Dichloropropane-d6	6.73	67	45233	4.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.00%
41) Toluene-d8	7.92	98	127211	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	8.20	79	18496	4.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.40%
46) 2-Hexanone-d5	8.66	63	81704	50.57	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.14%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	36561	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.60%
64) 1,2-Dichlorobenzene-d4	12.21	152	45287	5.09	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.80%


Target Compounds					Ovalue
13) Acetone	2.66	43	2583	1.530 ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031320\
Data File : VU037249.D
Acq On : 13 Mar 2020 18:11
Operator : JC/MD
Sample : L1900-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONB9

Quant Time: Mar 14 01:28:34 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 14 00:24:25 2020
Response via : Initial Calibration

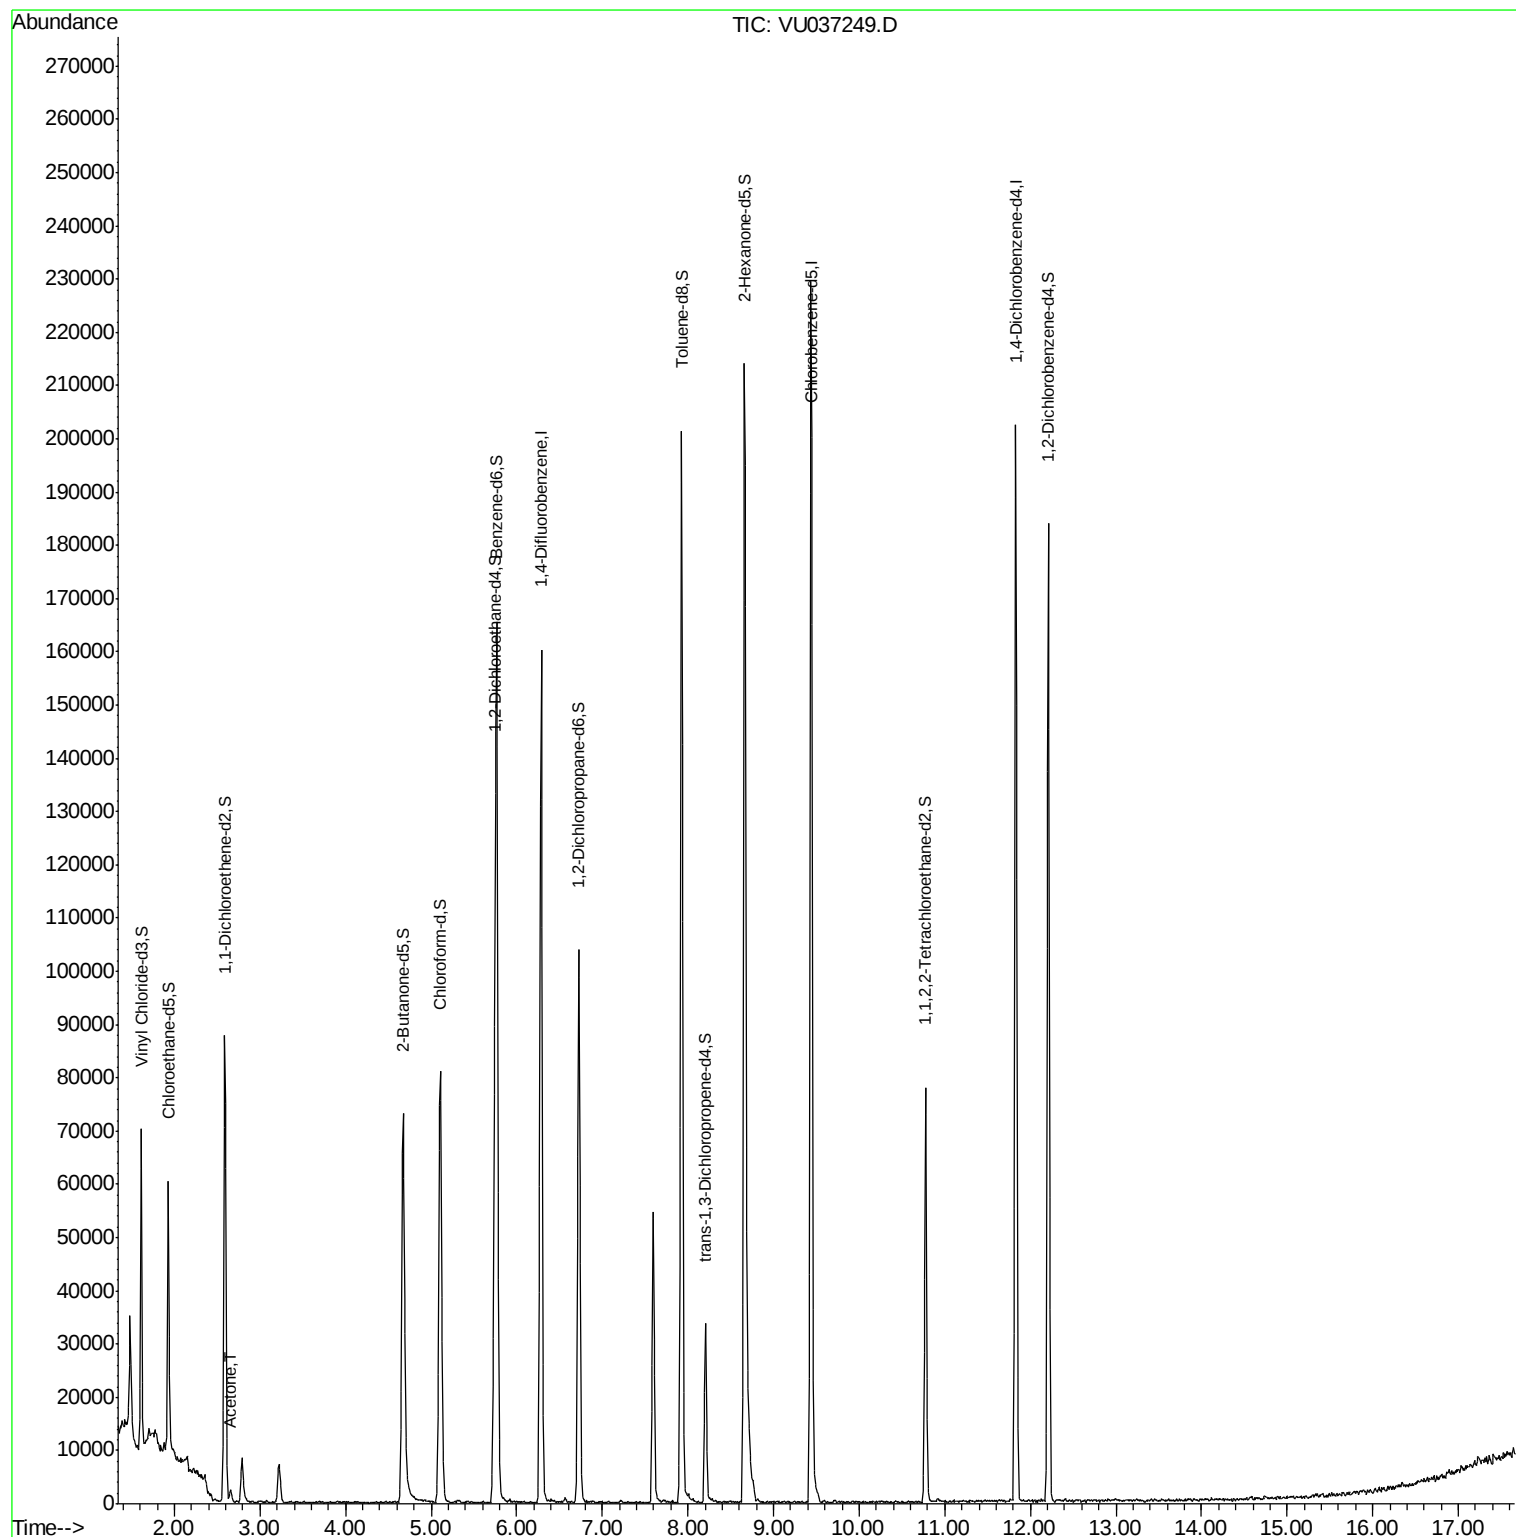

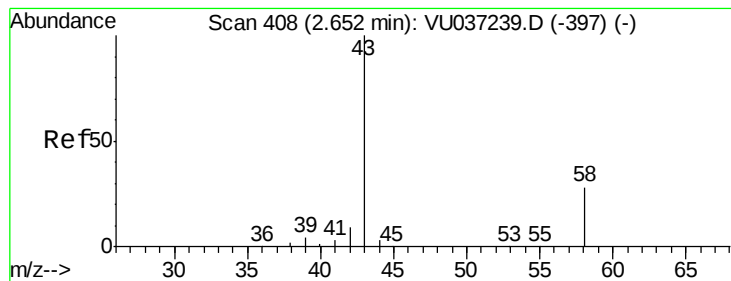

#13

Acetone

Concen: 1.530 ug/L

RT: 2.66 min Scan# 409

Delta R.T. 0.00 min

Lab File: VU037249.D

Acq: 13 Mar 2020 18:11

Instrument :
MSVOA_U
ClientSampleId :
CONB9

Tot Ion: 43 Resp: 2583

Ion Ratio Lower Upper

43 100

58 13.3 0.0 52.2

