

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031320\
 Data File : VU037251.D
 Acq On : 13 Mar 2020 19:01
 Operator : JC/MD
 Sample : L1900-11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COND2

Quant Time: Mar 14 01:37:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 14 00:24:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	121217	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	121081	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	49890	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	37408	4.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.00%
7) Chloroethane-d5	1.93	69	32384	5.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	115.20%
11) 1,1-Dichloroethene-d2	2.59	63	51383	3.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.60%
20) 2-Butanone-d5	4.67	46	100277	49.25	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.50%
24) Chloroform-d	5.11	84	75165	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.74	65	45600	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.76	84	137135	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
36) 1,2-Dichloropropane-d6	6.73	67	44214	4.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.80%
41) Toluene-d8	7.92	98	123226	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.40%
43) trans-1,3-Dichloropropene-	8.20	79	18756	4.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.60%
46) 2-Hexanone-d5	8.66	63	76641	47.37	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.74%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	35110	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.80%
64) 1,2-Dichlorobenzene-d4	12.21	152	44346	5.15	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.00%


Target Compounds					Ovalue
13) Acetone	2.65	43	3537	2.120 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031320\
Data File : VU037251.D
Acq On : 13 Mar 2020 19:01
Operator : JC/MD
Sample : L1900-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COND2

Quant Time: Mar 14 01:37:34 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 14 00:24:25 2020
Response via : Initial Calibration

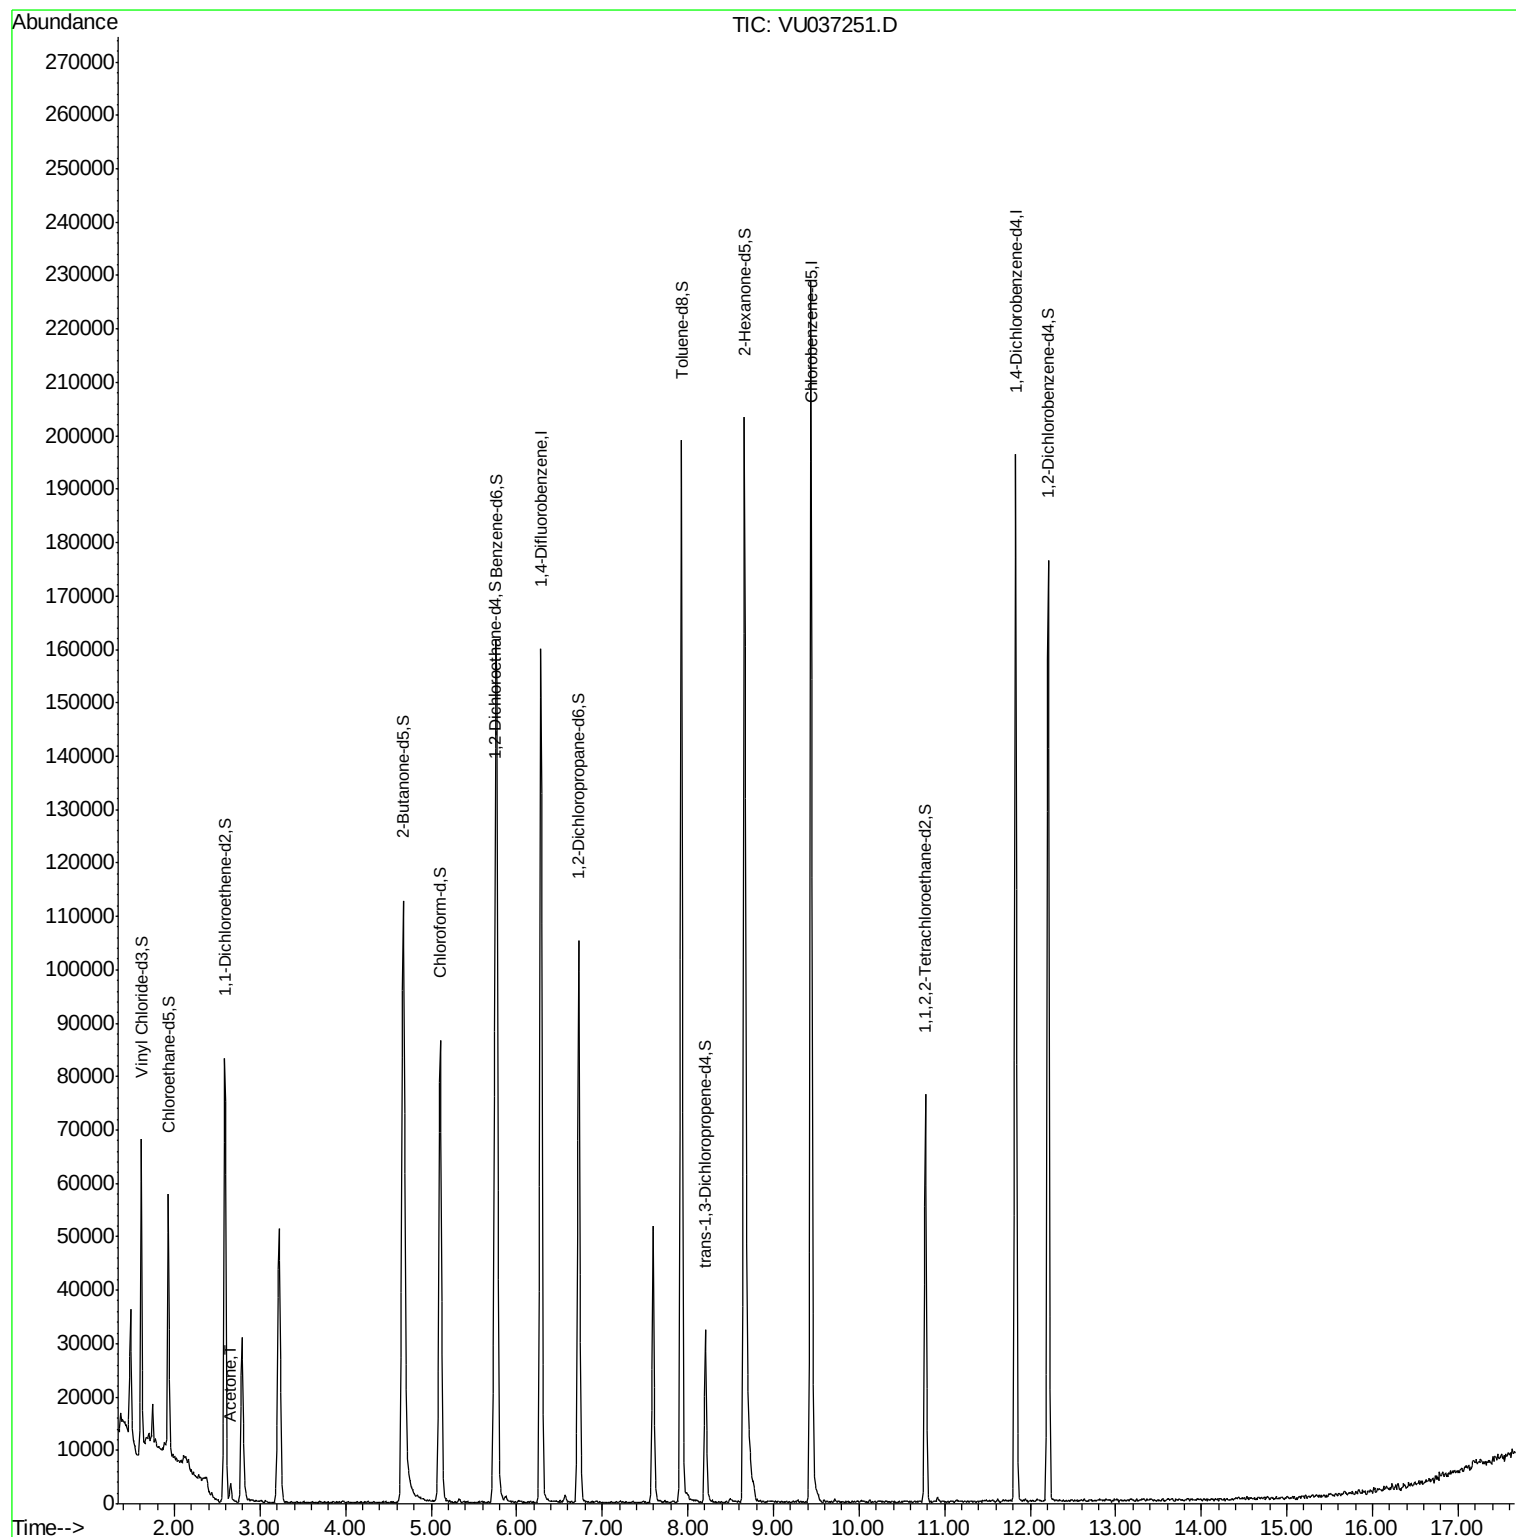

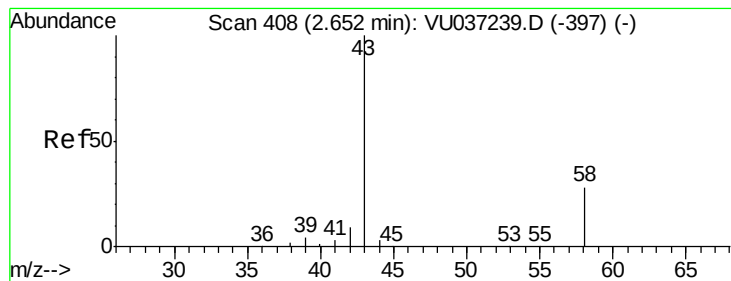

#13

Acetone

Concen: 2.120 ug/L

RT: 2.65 min Scan# 409

Delta R.T. 0.00 min

Lab File: VU037251.D

Acq: 13 Mar 2020 19:01

Instrument :
MSVOA_U
ClientSampleId :
COND2

Tot Ion: 43 Resp: 3537

Ion Ratio Lower Upper

43 100

58 27.1 0.0 52.2

