


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031320\
 Data File : VU037238.D
 Acq On : 13 Mar 2020 12:52
 Operator : JC/MD
 Sample : BFB03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB03

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Mar 16 06:54:28 2020

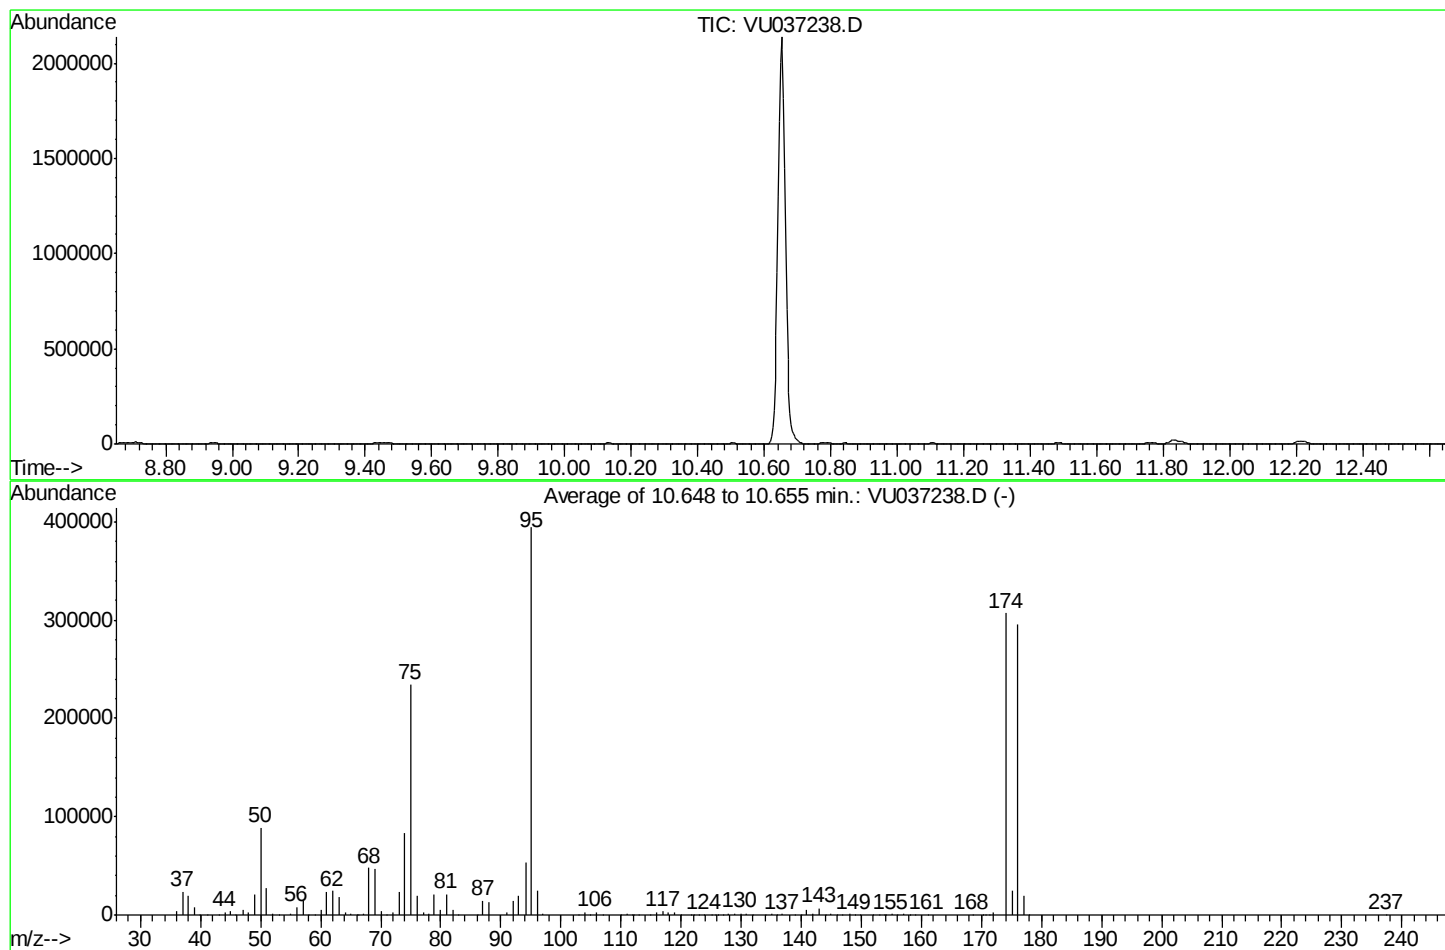

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	89008	PASS
75	95	30	80	59.3	233920	PASS
95	95	100	100	100.0	394346	PASS
96	95	5	9	6.4	25360	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.8	306965	PASS
175	174	5	9	8.0	24418	PASS
176	174	95	101	96.1	295104	PASS
177	176	5	9	6.8	19949	PASS

Scan 2880 (10.600 min): VU037238.D
BFB02

m/z	Abundance
39.90	219.0
44.00	598.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	4222.0
37.00	24056.0
38.00	20128.0
39.00	7779.0
40.00	431.0
41.20	100.0
43.00	432.0
44.00	3677.0
45.00	3957.0
45.90	491.0
47.00	4739.0
48.00	2829.0
49.00	19944.0
50.00	87464.0
51.00	26752.0
52.00	1393.0
53.10	283.0
55.00	1202.0
56.00	7795.0
57.00	13514.0
58.00	722.0
59.10	141.0
60.00	4603.0
61.00	23200.0
62.00	24512.0
63.00	17552.0
64.00	2254.0
65.00	2064.0
66.00	174.0
67.10	1402.0
68.00	46296.0
69.00	46096.0
70.00	3401.0
71.00	174.0
72.00	2641.0
73.00	22072.0
74.00	80472.0
75.00	226240.0
76.00	18864.0
77.10	2755.0
77.90	1866.0
78.90	20504.0
79.90	5760.0
80.90	19992.0
81.90	4608.0
82.90	606.0
86.10	594.0
87.00	13886.0
88.00	13292.0
90.90	2379.0
92.00	13385.0
93.00	18896.0
94.10	53488.0
95.10	385856.0
96.10	24824.0
97.00	879.0
102.90	165.0
103.90	2324.0
104.90	523.0
105.90	2842.0
106.90	384.0
109.90	435.0
111.00	585.0
111.80	329.0
112.00	332.0
112.90	512.0
114.90	556.0
115.90	1885.0
117.00	3773.0
117.90	1875.0
119.00	2966.0
120.00	205.0
122.20	106.0
123.00	213.0
123.90	264.0
125.90	194.0
126.90	121.0
127.90	1486.0
128.90	815.0
129.90	1752.0
130.90	698.0
131.90	102.0
133.90	157.0
135.00	878.0
136.00	172.0
136.80	747.0
139.00	161.0
140.00	528.0
141.00	5324.0
141.90	731.0
143.00	6623.0
144.00	486.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

145.00	1183.0
145.90	594.0
146.80	298.0
148.00	1219.0
148.80	266.0
149.90	367.0
151.90	159.0
153.10	287.0
154.10	272.0
155.10	998.0
156.00	228.0
157.10	791.0
158.10	140.0
159.00	476.0
161.00	512.0
170.20	159.0
170.80	390.0
171.30	508.0
172.00	2108.0
174.10	289344.0
175.10	23184.0
176.10	279360.0
177.10	19400.0
178.00	582.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	4596.0
37.00	24792.0
38.00	20552.0
39.10	8030.0
40.00	422.0
43.00	349.0
44.00	3878.0
45.00	4219.0
45.90	451.0
47.00	5054.0
48.00	3129.0
49.00	20968.0
50.00	92112.0
51.00	27680.0
52.00	1334.0
53.10	279.0
55.00	1382.0
56.00	8144.0
57.00	14206.0
58.00	648.0
59.10	135.0
60.00	4943.0
61.00	24608.0
62.00	25296.0
63.00	18912.0
64.10	2094.0
65.00	1874.0
66.20	173.0
67.00	1430.0
68.00	49144.0
69.00	49032.0
70.00	3629.0
71.00	186.0
72.00	2927.0
73.00	23760.0
74.00	86280.0
75.00	242368.0
76.10	20080.0
77.10	2761.0
78.00	2026.0
78.90	20856.0
80.00	6022.0
80.90	21864.0
81.90	4829.0
82.90	614.0
86.00	657.0
87.00	15308.0
88.00	14155.0
90.90	2285.0
92.00	14368.0
93.00	20736.0
94.10	55696.0
95.10	406848.0
96.10	26112.0
97.00	883.0
102.90	203.0
103.90	2682.0
104.90	604.0
105.90	3059.0
106.90	397.0
109.90	561.0
111.00	788.0
111.80	398.0
112.90	470.0
115.00	591.0
115.90	2213.0
117.00	3827.0
117.90	2025.0
119.00	3163.0
120.10	259.0
123.00	162.0
124.00	264.0
125.00	121.0
126.10	174.0
126.90	217.0
127.90	1655.0
128.90	831.0
129.90	1968.0
130.90	801.0
134.00	127.0
135.00	973.0
136.00	205.0
136.90	903.0
138.90	198.0
140.10	597.0
140.90	5860.0
141.90	731.0
143.00	7464.0
144.00	449.0
145.00	1060.0
145.90	661.0
146.80	314.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

148.00	1291.0
148.80	316.0
149.80	393.0
151.90	175.0
153.00	319.0
154.10	290.0
155.10	1165.0
155.90	211.0
157.10	716.0
158.10	135.0
159.00	487.0
161.00	598.0
168.50	113.0
170.20	179.0
170.80	331.0
172.10	2071.0
174.10	316992.0
175.10	25144.0
176.10	303744.0
177.10	20688.0
178.00	578.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	4471.0
37.00	22720.0
38.00	19248.0
39.10	7502.0
40.00	381.0
43.10	263.0
44.00	3621.0
45.00	4037.0
47.00	4608.0
48.00	3054.0
49.00	20280.0
50.00	87448.0
51.00	25912.0
52.00	1093.0
53.10	226.0
55.00	1554.0
56.00	7896.0
57.00	13509.0
58.00	503.0
60.00	4882.0
61.00	23528.0
62.00	23456.0
63.00	18352.0
64.10	1739.0
65.00	1595.0
66.20	149.0
67.00	1331.0
68.00	47272.0
69.00	47528.0
70.00	3538.0
71.10	203.0
72.00	2813.0
73.00	22744.0
74.00	82760.0
75.00	233152.0
76.10	19312.0
77.10	2470.0
78.00	1826.0
78.90	19368.0
80.00	5867.0
80.90	21344.0
82.00	4850.0
82.90	577.0
86.00	583.0
87.00	15263.0
88.00	13560.0
90.90	1950.0
92.00	14174.0
93.00	20376.0
94.10	52520.0
95.10	390336.0
96.10	25144.0
97.00	748.0
102.90	211.0
103.90	2701.0
104.90	651.0
105.90	2854.0
106.90	370.0
109.90	552.0
111.00	888.0
111.80	429.0
112.90	431.0
115.00	608.0
115.90	2304.0
117.00	3543.0
117.90	2218.0
119.00	3024.0
120.10	206.0
121.60	173.0
123.00	130.0
123.80	288.0
125.00	140.0
125.70	127.0
126.10	129.0
126.90	268.0
127.90	1727.0
129.00	790.0
129.90	1996.0
130.90	707.0
134.10	102.0
135.00	984.0
135.90	200.0
136.90	978.0
138.90	233.0
140.10	552.0
140.90	5832.0
142.00	723.0
143.00	7416.0
143.90	381.0
145.00	823.0
145.90	740.0
146.80	304.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

148.00	1111.0
148.90	383.0
149.80	424.0
151.90	191.0
153.00	370.0
153.80	306.0
155.00	1157.0
156.00	170.0
157.00	673.0
158.00	123.0
159.10	470.0
161.00	539.0
170.20	187.0
170.70	260.0
172.10	2073.0
174.10	314560.0
175.10	24928.0
176.10	302208.0
177.10	19760.0
178.00	548.0
237.40	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03