

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
 Data File : VU042635.D
 Acq On : 13 Mar 2021 02:00
 Operator : SY/MD
 Sample : M1676-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD5

Quant Time: Mar 13 06:44:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Mar 13 06:39:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	76507	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	75532	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	34053	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	21665	4.25	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.00%
7) Chloroethane-d5	1.919	69	20481	5.30	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.00%
11) 1,1-Dichloroethene-d2	2.575	63	36036	3.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.60%
20) 2-Butanone-d5	4.642	46	81852	48.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.76%
24) Chloroform-d	5.073	84	49581	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
26) 1,2-Dichloroethane-d4	5.710	65	32913	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.00%
32) Benzene-d6	5.735	84	89925	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
36) 1,2-Dichloropropane-d6	6.700	67	29342	4.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.20%
41) Toluene-d8	7.906	98	83958	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
43) trans-1,3-Dichloroprop...	8.189	79	10891	3.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.00%
46) 2-Hexanone-d5	8.645	63	59573	44.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.16%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	25270	4.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.00%
64) 1,2-Dichlorobenzene-d4	12.201	152	32499	5.26	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.20%
Target Compounds						Qvalue
22) cis-1,2-Dichloroethene	4.674	96	1150	0.19	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042635.D
Acq On : 13 Mar 2021 02:00
Operator : SY/MD
Sample : M1676-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD5

Quant Time: Mar 13 06:44:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Mar 13 06:39:26 2021
Response via : Initial Calibration

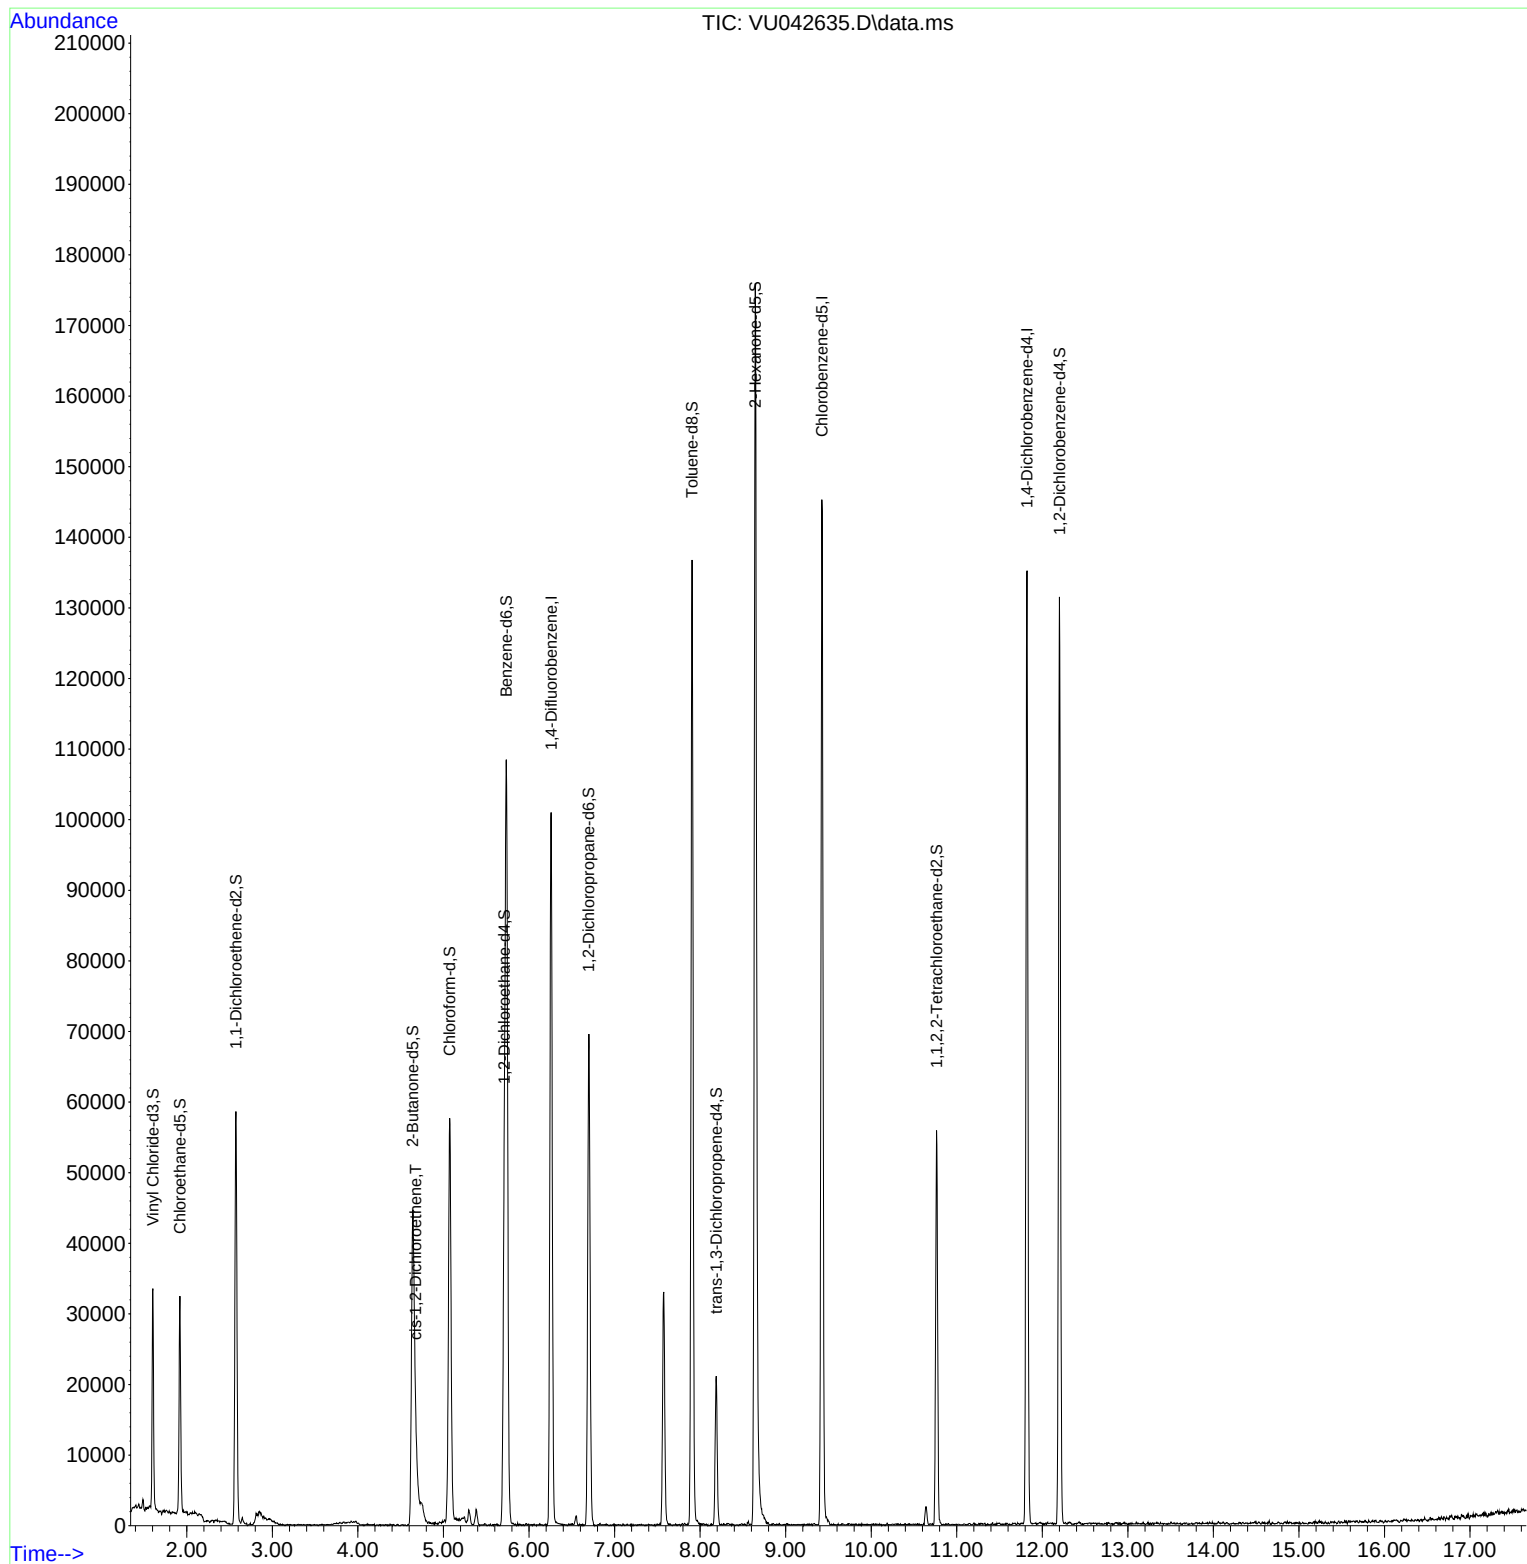

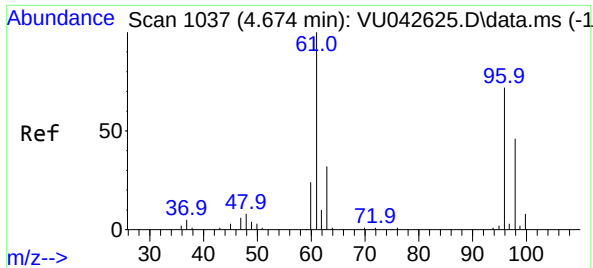

cis-1,2-Dichloroethene
 Concen: 0.19 ug/L
 RT: 4.674 min Scan# 1037
 Delta R.T. -0.000 min
 Lab File: VU042635.D
 Acq: 13 Mar 2021 02:00

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD5

Tgt Ion: 96	Resp: 1150
Ion Ratio	Lower Upper
96 100	
61 149.1	97.8 181.6
68 0.0	0.0 0.0

