

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
 Data File : VU042608.D
 Acq On : 12 Mar 2021 14:15
 Operator : SY/MD
 Sample : M1674-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BD3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042608.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	94	rVB	33515	38291	11.03%	1.492%
2	1.919	172	180	193	rVB	29088	37521	10.81%	1.462%
3	2.575	373	384	398	rBV2	64231	105314	30.33%	4.104%
4	4.649	1013	1029	1069	rBV	31998	130921	37.70%	5.102%
5	5.073	1147	1161	1181	rBV2	56300	122858	35.38%	4.788%
6	5.298	1221	1231	1242	rBV3	2661	4783	1.38%	0.186%
7	5.382	1247	1257	1269	rVB4	3285	5810	1.67%	0.226%
8	5.736	1346	1367	1384	rBV2	108906	286544	82.52%	11.167%
9	6.256	1516	1529	1552	rBV	106829	204258	58.82%	7.960%
10	6.700	1653	1667	1683	rBV2	71099	137133	39.49%	5.344%
11	7.575	1927	1939	1953	rBV	34985	61789	17.79%	2.408%
12	7.906	2028	2042	2057	rBV	138172	239837	69.07%	9.347%
13	8.189	2119	2130	2144	rBV2	21837	38168	10.99%	1.487%
14	8.645	2257	2272	2305	rBV	158626	347241	100.00%	13.532%
15	9.424	2499	2514	2537	rBV	153013	259388	74.70%	10.109%
16	10.639	2885	2892	2901	rBV3	3876	5257	1.51%	0.205%
17	10.764	2919	2931	2950	rVB2	55661	89375	25.74%	3.483%
18	11.819	3247	3259	3276	rVB	147295	236315	68.06%	9.209%
19	12.202	3361	3378	3392	rBV	132610	215194	61.97%	8.386%




Sum of corrected areas: 2565997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042608.D
Acq On : 12 Mar 2021 14:15
Operator : SY/MD
Sample : M1674-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

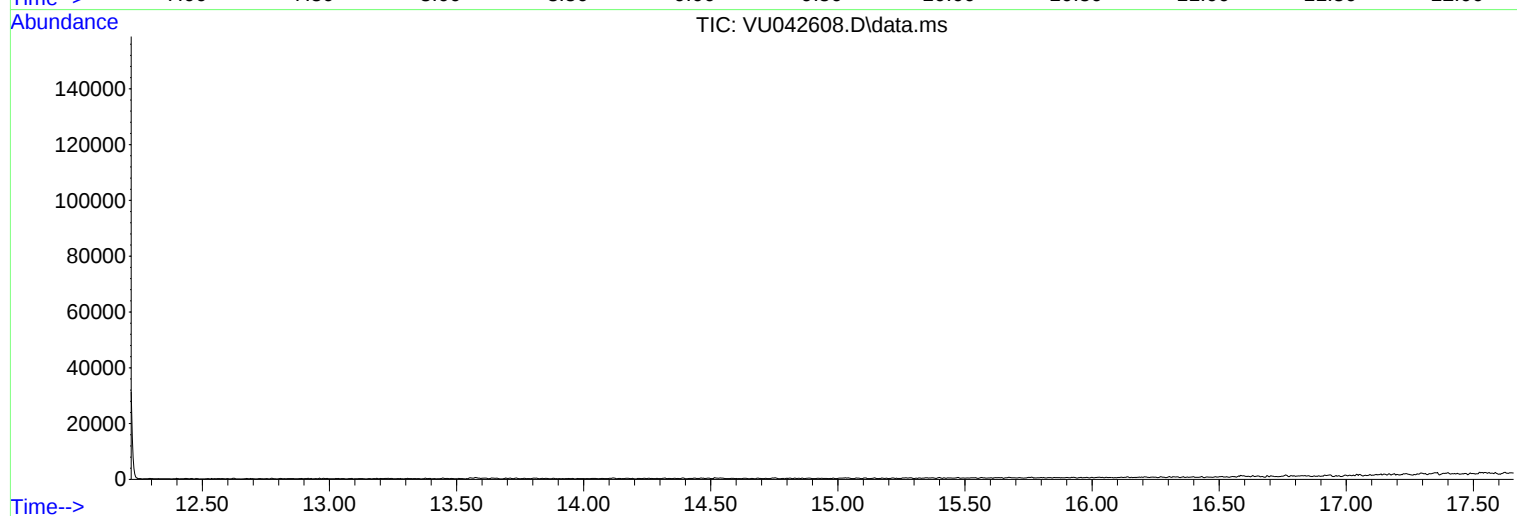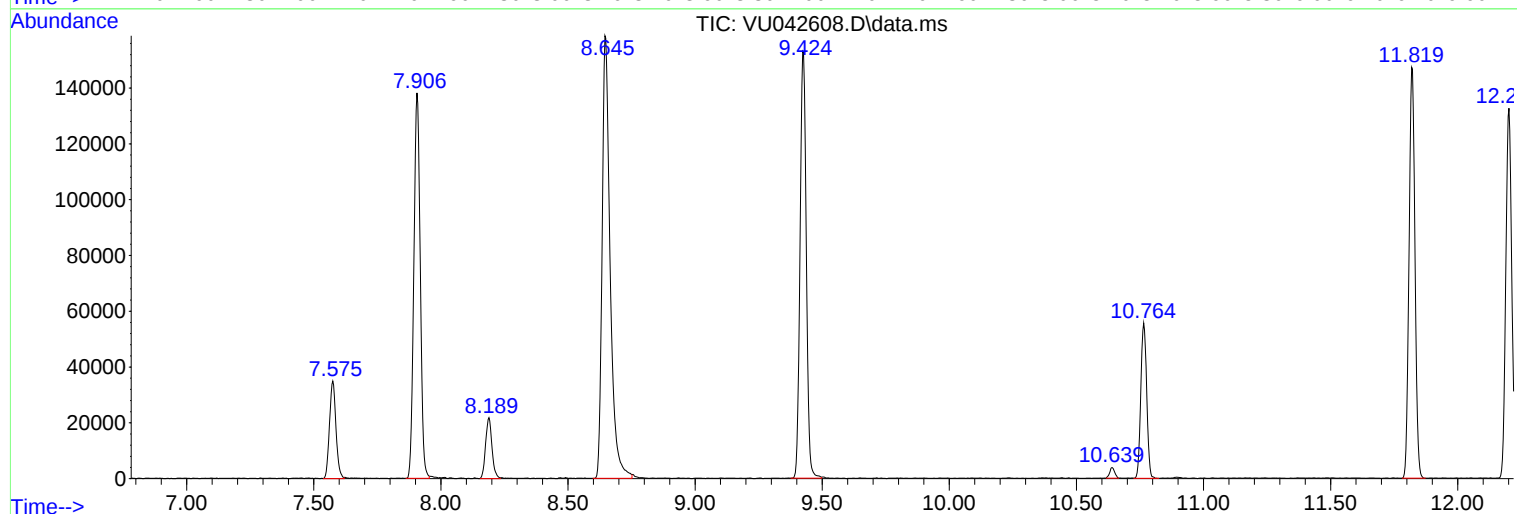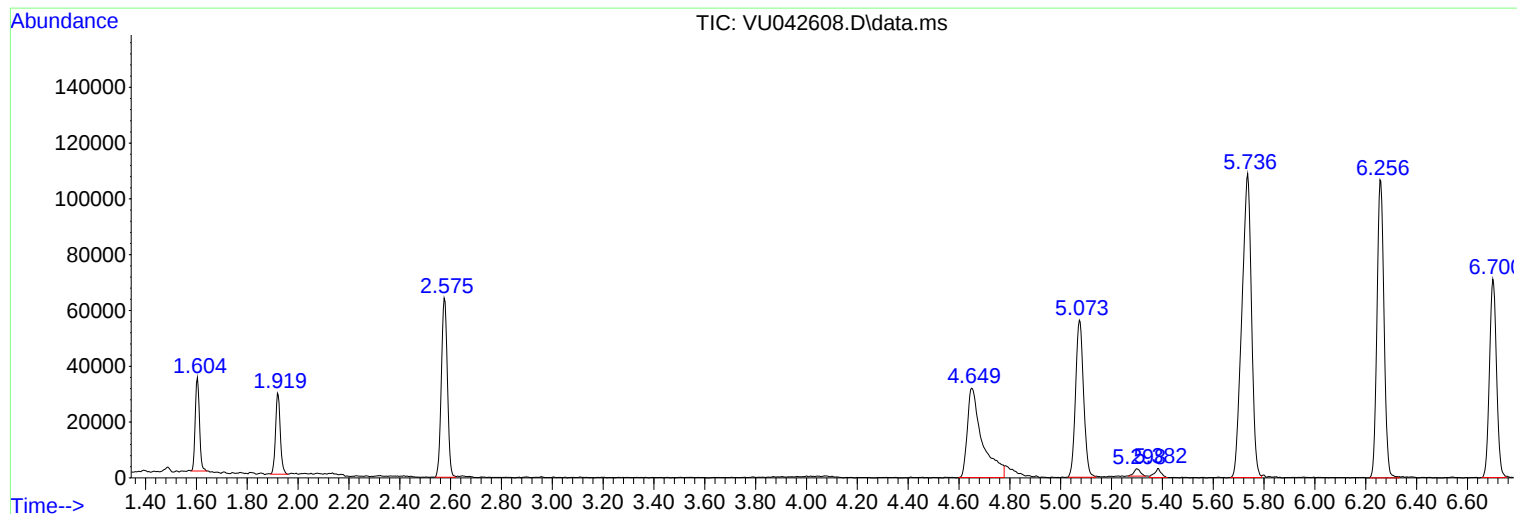

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042608.D
Acq On : 12 Mar 2021 14:15
Operator : SY/MD
Sample : M1674-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042608.D
Acq On : 12 Mar 2021 14:15
Operator : SY/MD
Sample : M1674-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
