

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
 Data File : VU042626.D
 Acq On : 12 Mar 2021 22:23
 Operator : SY/MD
 Sample : VU0313WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK27

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042626.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rVB	33539	39900	11.54%	1.579%
2	1.919	172	180	190	rVB	30618	38753	11.21%	1.534%
3	2.575	372	384	396	rBV	67017	108834	31.48%	4.308%
4	3.054	523	533	543	rBV3	2270	4172	1.21%	0.165%
5	4.648	1014	1029	1067	rBV2	33064	128290	37.11%	5.078%
6	5.073	1147	1161	1184	rBV	57667	125116	36.19%	4.953%
7	5.298	1221	1231	1242	rVB4	2175	4121	1.19%	0.163%
8	5.378	1248	1256	1267	rVB3	2102	4212	1.22%	0.167%
9	5.735	1347	1367	1387	rBV3	110476	294328	85.14%	11.651%
10	6.256	1515	1529	1546	rBV	99175	188017	54.39%	7.443%
11	6.700	1652	1667	1692	rBV	68992	138286	40.00%	5.474%
12	7.574	1928	1939	1953	rBV2	33870	60179	17.41%	2.382%
13	7.906	2029	2042	2060	rBV	139070	240926	69.70%	9.537%
14	8.185	2119	2129	2149	rVB2	21862	36842	10.66%	1.458%
15	8.645	2260	2272	2303	rBV	163123	345686	100.00%	13.684%
16	9.423	2502	2514	2530	rBV	144997	241200	69.77%	9.548%
17	10.642	2885	2893	2901	rVB3	3229	4692	1.36%	0.186%
18	10.764	2920	2931	2945	rVB	56269	90533	26.19%	3.584%
19	11.819	3246	3259	3275	rBV	135970	217542	62.93%	8.612%
20	12.201	3366	3378	3394	rBV	133537	214518	62.06%	8.492%




Sum of corrected areas: 2526147

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042626.D
Acq On : 12 Mar 2021 22:23
Operator : SY/MD
Sample : VU0313WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

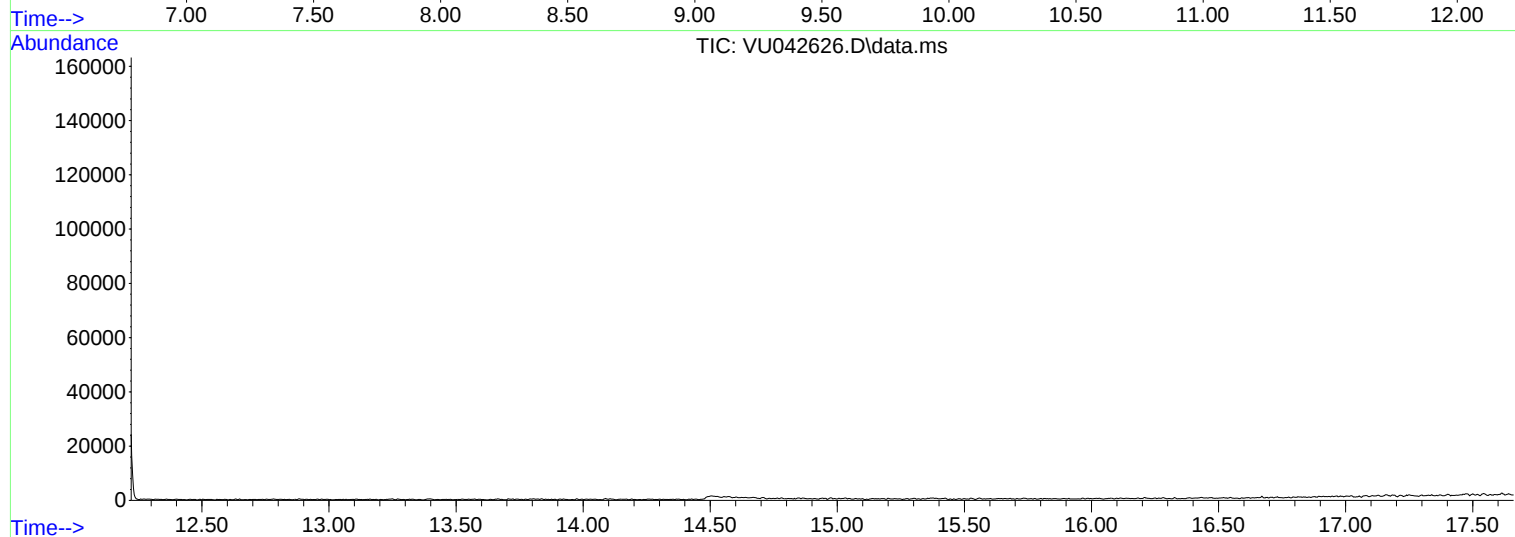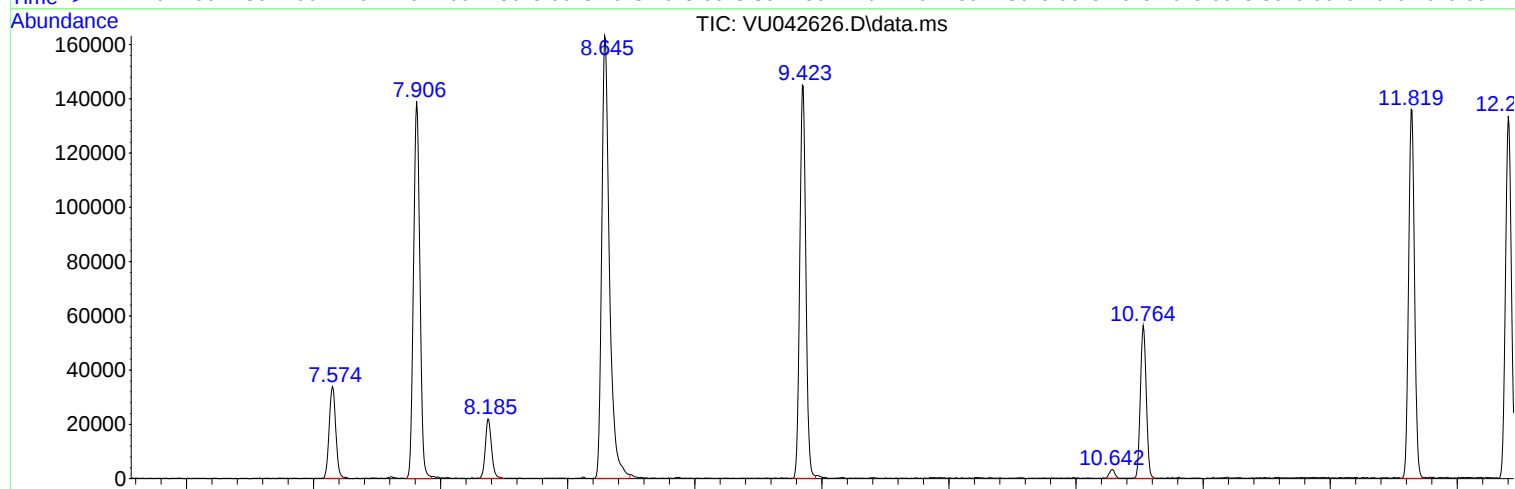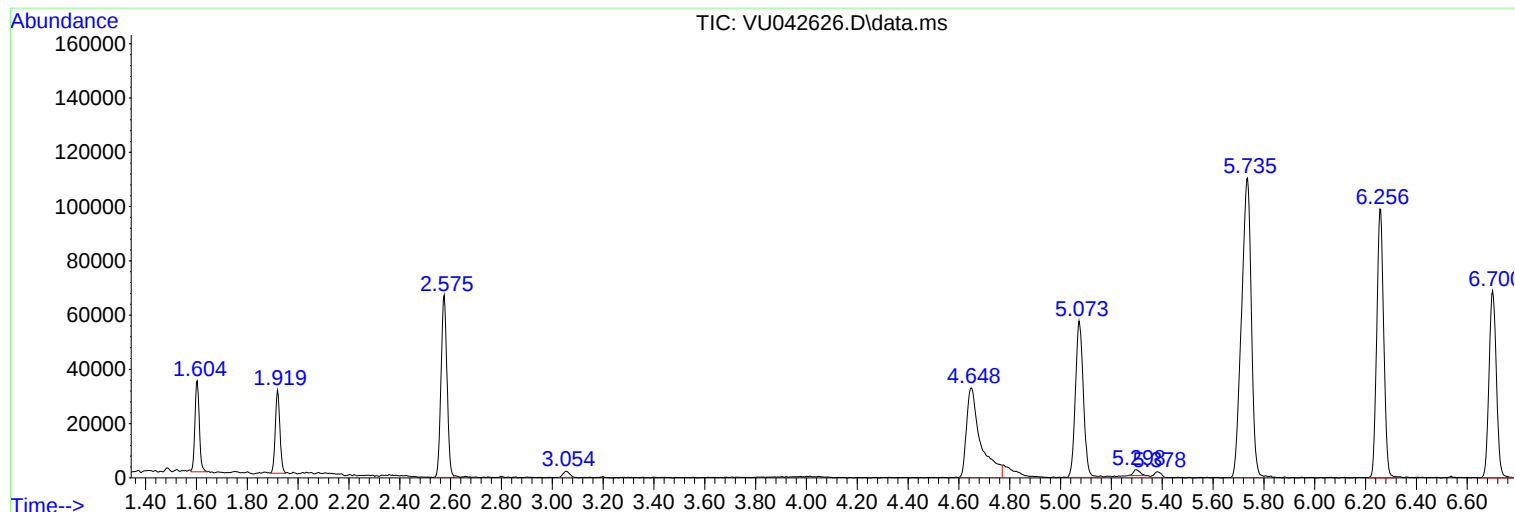

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042626.D
Acq On : 12 Mar 2021 22:23
Operator : SY/MD
Sample : VU0313WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042626.D
Acq On : 12 Mar 2021 22:23
Operator : SY/MD
Sample : VU0313WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
