

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
 Data File : VU042627.D
 Acq On : 12 Mar 2021 22:47
 Operator : SY/MD
 Sample : M1679-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AF3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC: VU042627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	95	rVB	32544	37459	11.58%	1.427%
2	1.919	170	180	193	rVB	30774	40544	12.53%	1.544%
3	2.575	373	384	401	rBV	58298	96332	29.78%	3.669%
4	2.806	444	456	458	rBV4	2460	3397	1.05%	0.129%
5	4.642	1010	1027	1060	rBV	41284	128892	39.85%	4.909%
6	5.073	1140	1161	1182	rBV	55484	121662	37.61%	4.634%
7	5.305	1220	1233	1241	rBV4	2348	4950	1.53%	0.189%
8	5.385	1250	1258	1267	rVB4	2057	3946	1.22%	0.150%
9	5.735	1345	1367	1385	rBV2	105115	282514	87.34%	10.760%
10	6.256	1516	1529	1545	rBV	104322	194216	60.04%	7.397%
11	6.700	1654	1667	1683	rBV2	69583	132325	40.91%	5.040%
12	7.575	1927	1939	1953	rBV2	31896	57644	17.82%	2.196%
13	7.906	2029	2042	2062	rBV	137440	234109	72.37%	8.917%
14	8.189	2119	2130	2144	rBV3	20871	34443	10.65%	1.312%
15	8.562	2234	2246	2260	rBV	102491	170347	52.66%	6.488%
16	8.645	2260	2272	2299	rBV	169407	323476	100.00%	12.321%
17	9.427	2501	2515	2530	rBV	144905	243806	75.37%	9.286%
18	10.639	2884	2892	2900	rBV5	3208	4340	1.34%	0.165%
19	10.764	2920	2931	2945	rBV2	54238	86512	26.74%	3.295%
20	11.819	3249	3259	3275	rBV	137114	220057	68.03%	8.382%
21	12.201	3366	3378	3397	rVB	127009	204511	63.22%	7.789%




Sum of corrected areas: 2625482

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042627.D
Acq On : 12 Mar 2021 22:47
Operator : SY/MD
Sample : M1679-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

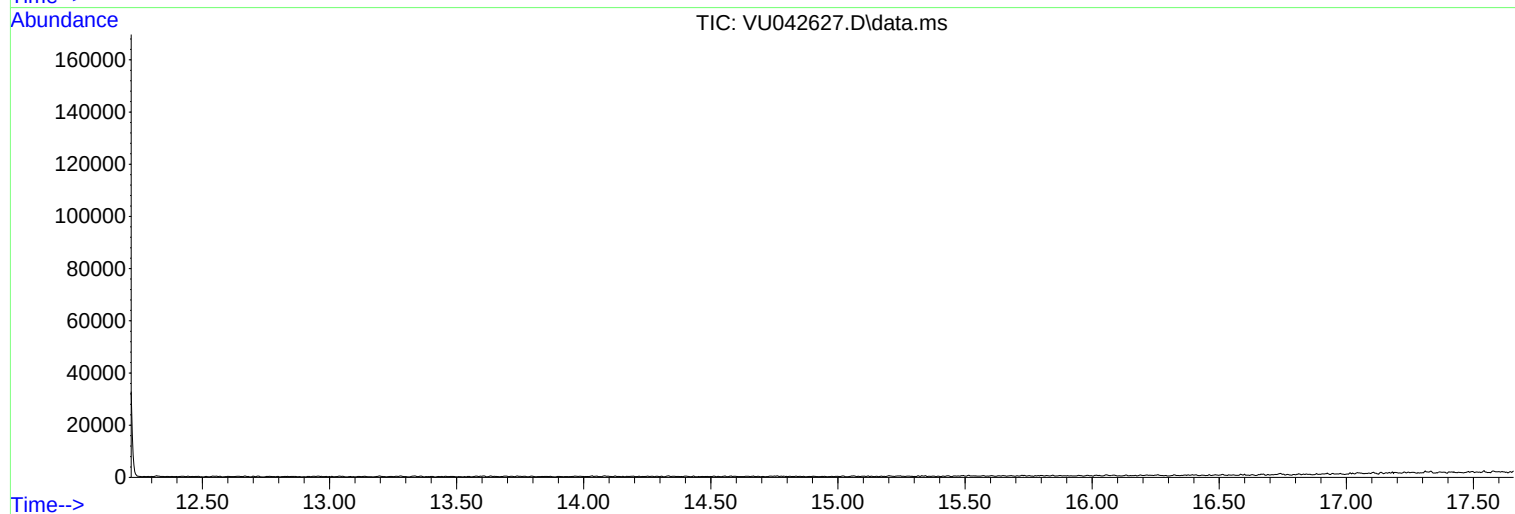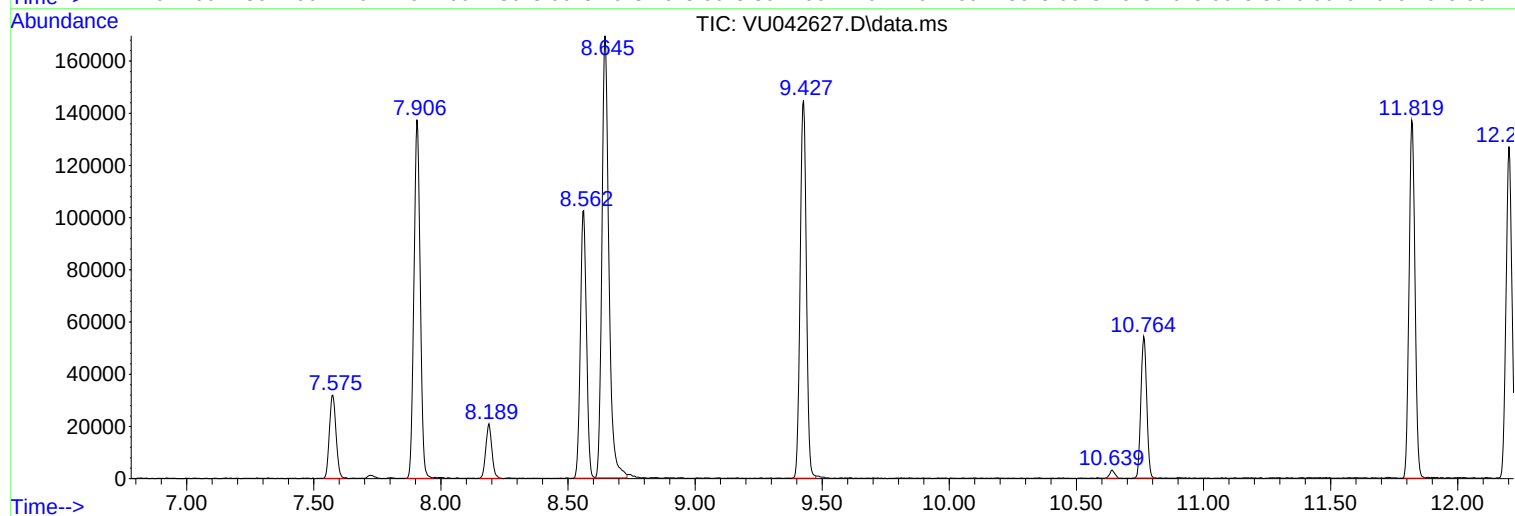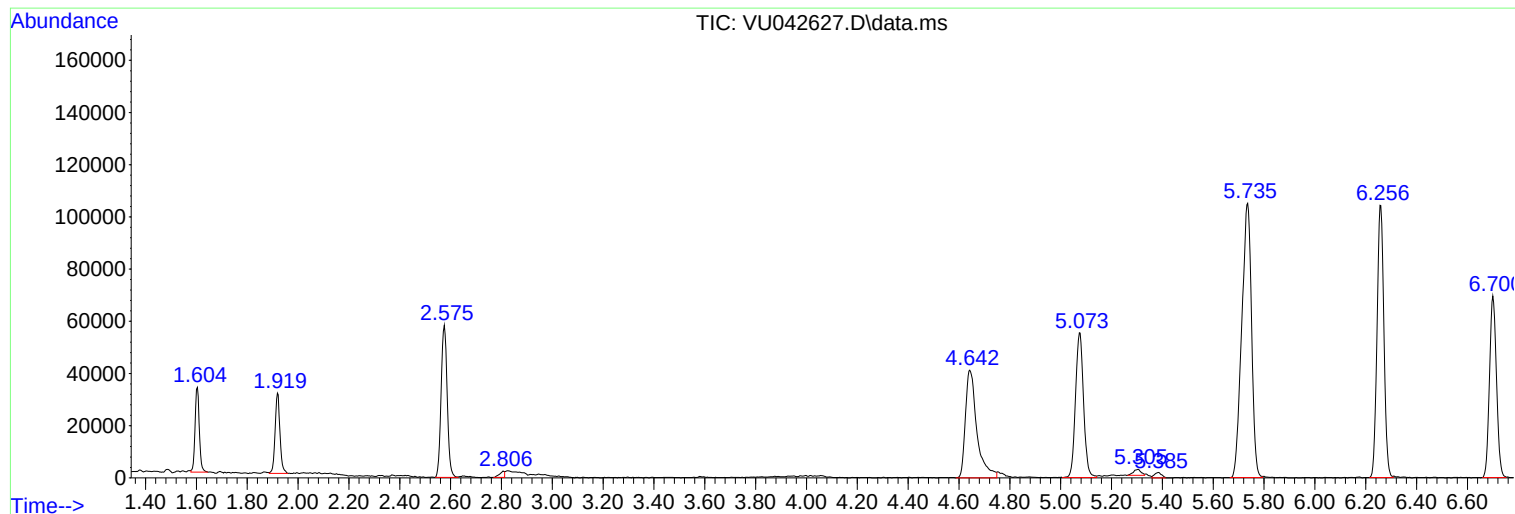

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042627.D
Acq On : 12 Mar 2021 22:47
Operator : SY/MD
Sample : M1679-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042627.D
Acq On : 12 Mar 2021 22:47
Operator : SY/MD
Sample : M1679-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
