

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
 Data File : VU042633.D
 Acq On : 13 Mar 2021 01:12
 Operator : SY/MD
 Sample : M1676-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042633.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	95	rVB	33039	39350	11.97%	1.608%
2	1.919	172	180	192	rVB	31535	41478	12.62%	1.695%
3	2.575	372	384	398	rBV	58350	94600	28.78%	3.866%
4	2.649	398	407	420	rVV3	2493	5052	1.54%	0.206%
5	2.832	442	464	468	rBV2	5187	13763	4.19%	0.562%
6	4.646	1012	1028	1050	rBV	42941	126462	38.47%	5.167%
7	5.073	1145	1161	1182	rBV	56647	133972	40.76%	5.474%
8	5.305	1222	1233	1247	rVV6	2349	5443	1.66%	0.222%
9	5.736	1345	1367	1390	rBV3	108291	287163	87.36%	11.734%
10	6.257	1516	1529	1548	rBV	100366	188128	57.23%	7.687%
11	6.700	1652	1667	1685	rBV	69805	133172	40.51%	5.442%
12	7.575	1928	1939	1959	rBV2	33687	59607	18.13%	2.436%
13	7.906	2029	2042	2060	rBV	136406	230380	70.09%	9.414%
14	8.189	2120	2130	2142	rBV3	20736	35062	10.67%	1.433%
15	8.646	2259	2272	2302	rBV	173076	328707	100.00%	13.432%
16	8.797	2311	2319	2330	rVB6	4946	8499	2.59%	0.347%
17	9.424	2502	2514	2527	rBV	141618	236041	71.81%	9.645%
18	10.642	2886	2893	2900	rBV3	2640	3564	1.08%	0.146%
19	10.764	2920	2931	2946	rBV	53588	85954	26.15%	3.512%
20	11.819	3247	3259	3273	rBV	124259	197663	60.13%	8.077%
21	12.202	3367	3378	3393	rVB	119782	193213	58.78%	7.895%




Sum of corrected areas: 2447273

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042633.D
Acq On : 13 Mar 2021 01:12
Operator : SY/MD
Sample : M1676-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

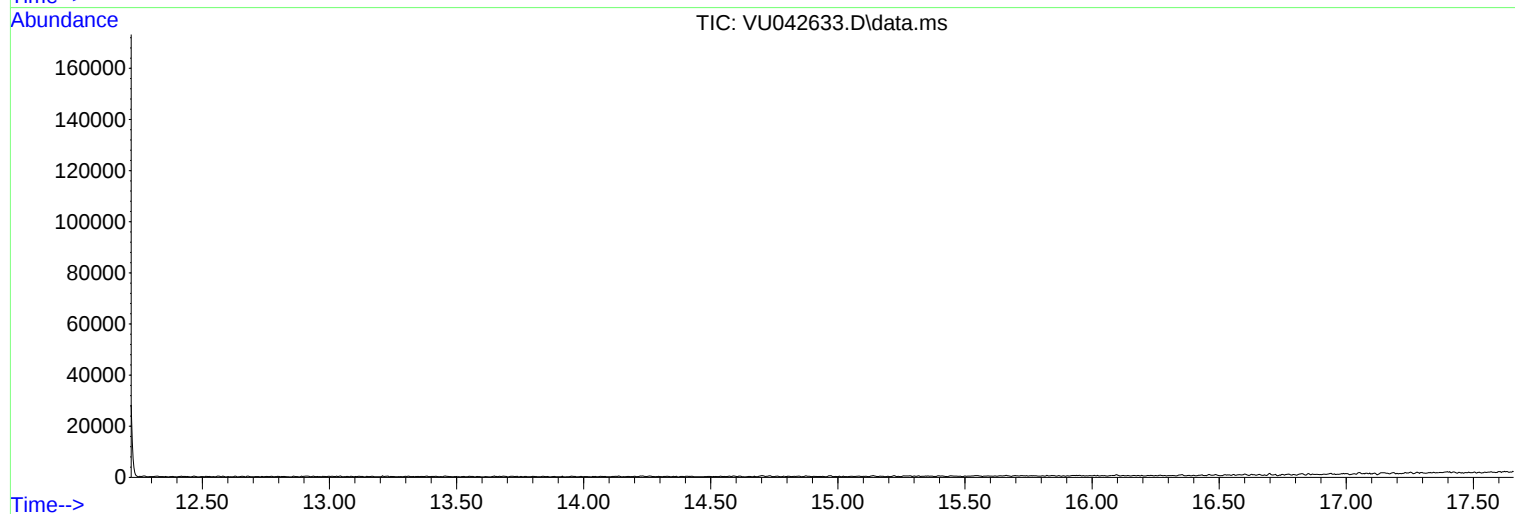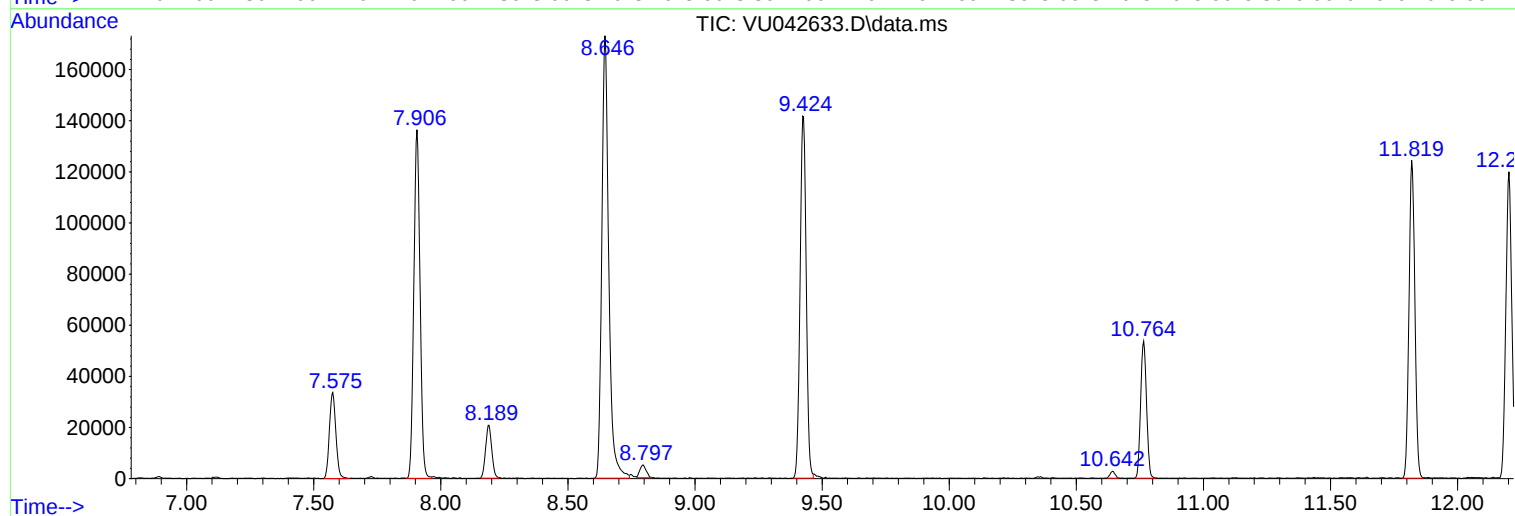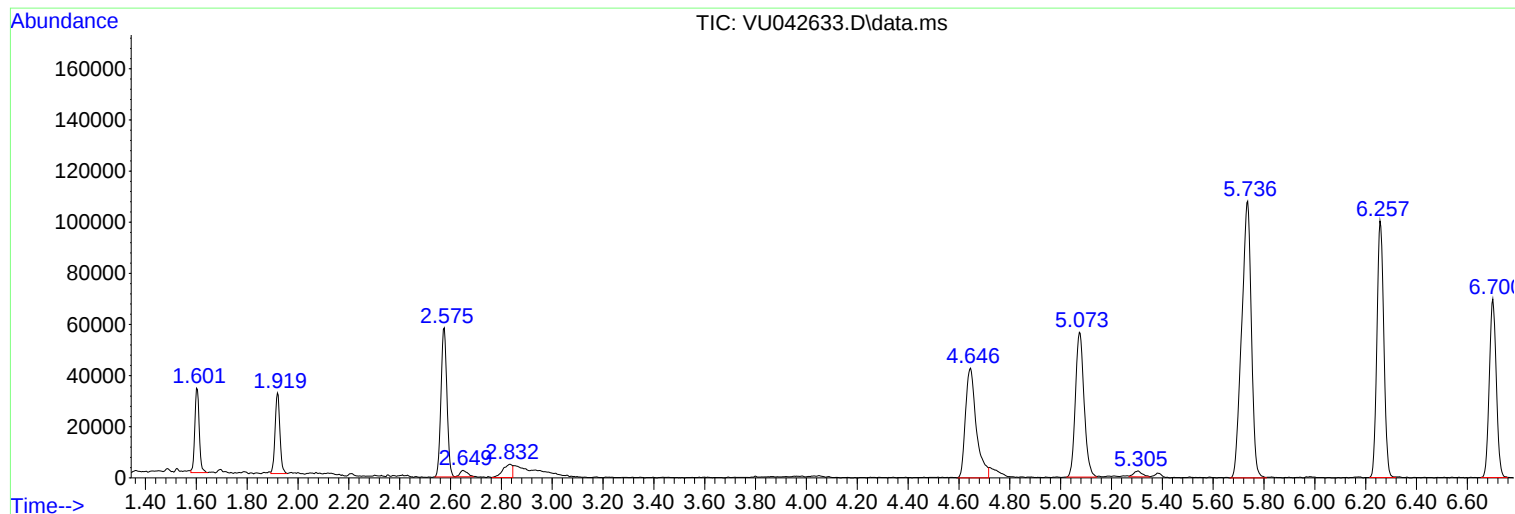

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042633.D
Acq On : 13 Mar 2021 01:12
Operator : SY/MD
Sample : M1676-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042633.D
Acq On : 13 Mar 2021 01:12
Operator : SY/MD
Sample : M1676-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
