

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
 Data File : VU042644.D
 Acq On : 13 Mar 2021 05:37
 Operator : SY/MD
 Sample : M1676-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AE4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC: VU042644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	93	rVB	31668	36593	10.64%	1.314%
2	1.919	172	180	192	rBV	29976	38804	11.28%	1.394%
3	2.575	372	384	397	rBV	57656	94025	27.33%	3.377%
4	2.829	448	463	465	rBV	2588	4765	1.39%	0.171%
5	4.642	1012	1027	1061	rBV	42163	133352	38.76%	4.789%
6	5.073	1143	1161	1178	rBV2	52718	117649	34.20%	4.225%
7	5.295	1222	1230	1248	rVB5	2825	6461	1.88%	0.232%
8	5.732	1345	1366	1385	rBV3	105574	283535	82.42%	10.183%
9	6.256	1516	1529	1547	rBV	100156	189039	54.95%	6.789%
10	6.700	1650	1667	1684	rBV2	68611	131915	38.35%	4.738%
11	7.575	1926	1939	1952	rBV	32686	56567	16.44%	2.032%
12	7.906	2029	2042	2057	rBV	132025	225042	65.42%	8.082%
13	8.189	2118	2130	2144	rBV3	19583	33352	9.70%	1.198%
14	8.559	2231	2245	2259	rBV	203264	344008	100.00%	12.355%
15	8.645	2259	2272	2297	rVV	174084	336206	97.73%	12.074%
16	9.423	2501	2514	2533	rBV	146765	244276	71.01%	8.773%
17	10.642	2885	2893	2901	rVB3	2542	3752	1.09%	0.135%
18	10.764	2917	2931	2944	rBV2	56261	88065	25.60%	3.163%
19	11.819	3248	3259	3276	rBV	135555	215880	62.75%	7.753%
20	12.202	3366	3378	3392	rBV	125738	201160	58.48%	7.224%




Sum of corrected areas: 2784446

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042644.D
Acq On : 13 Mar 2021 05:37
Operator : SY/MD
Sample : M1676-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

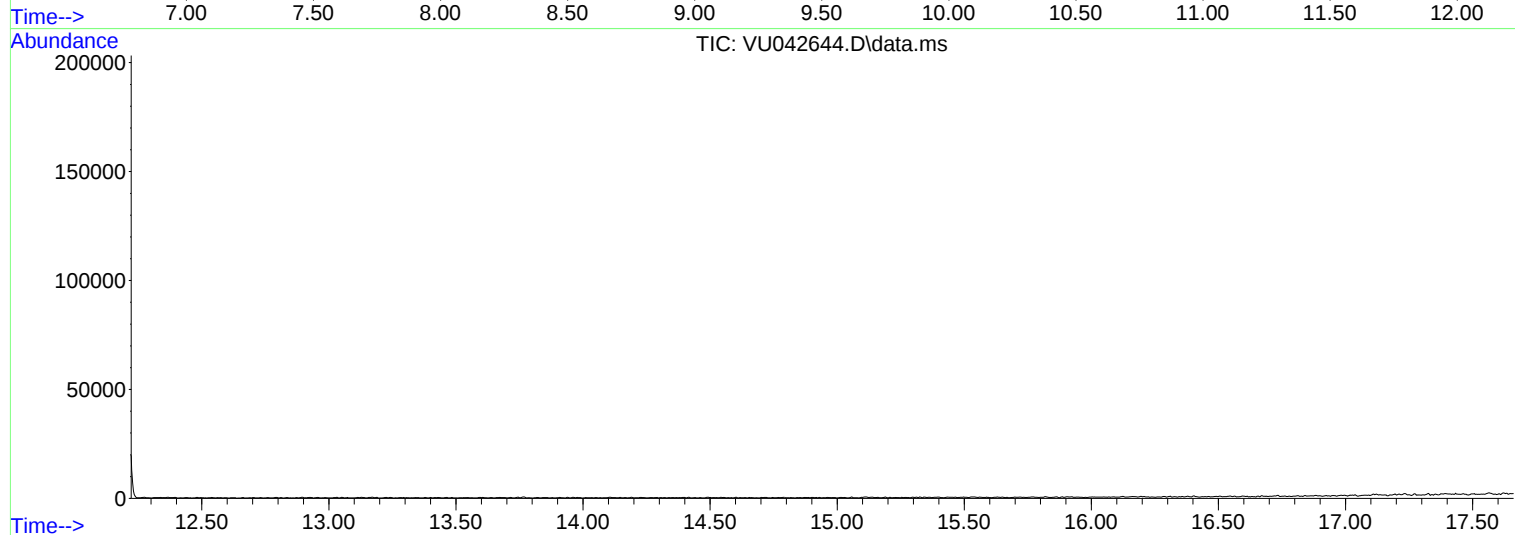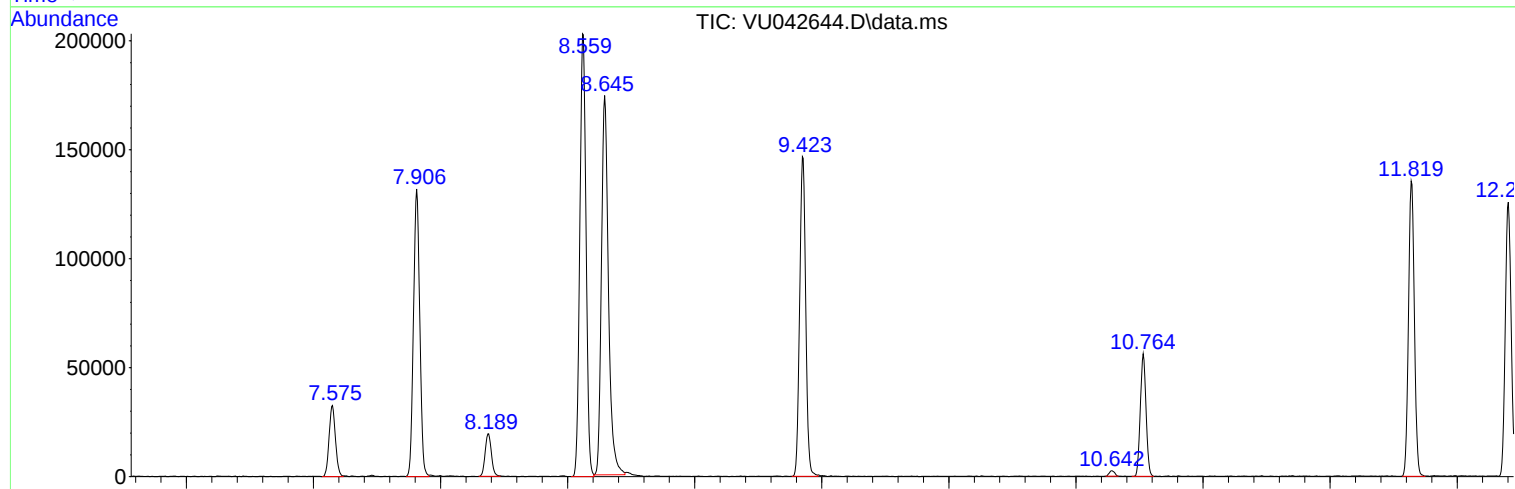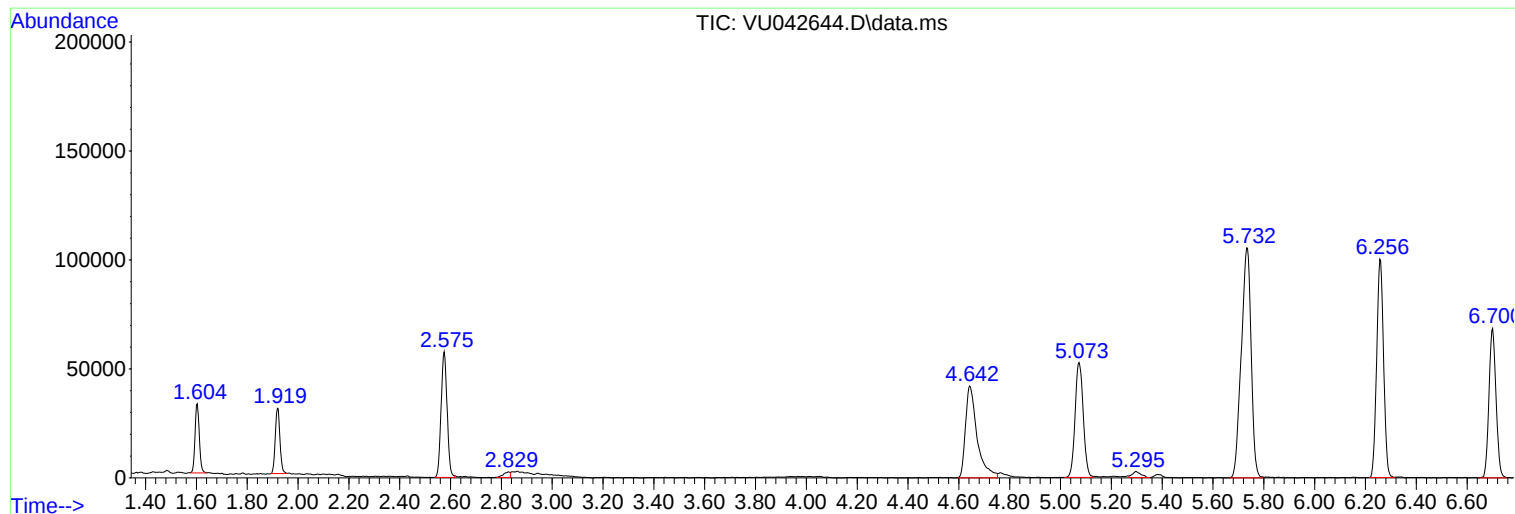

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042644.D
Acq On : 13 Mar 2021 05:37
Operator : SY/MD
Sample : M1676-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
Data File : VU042644.D
Acq On : 13 Mar 2021 05:37
Operator : SY/MD
Sample : M1676-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
