


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031321\
 Data File : VU042603.D
 Acq On : 12 Mar 2021 11:14
 Operator : SY/MD
 Sample : BFB25
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB25

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Mar 13 06:39:26 2021

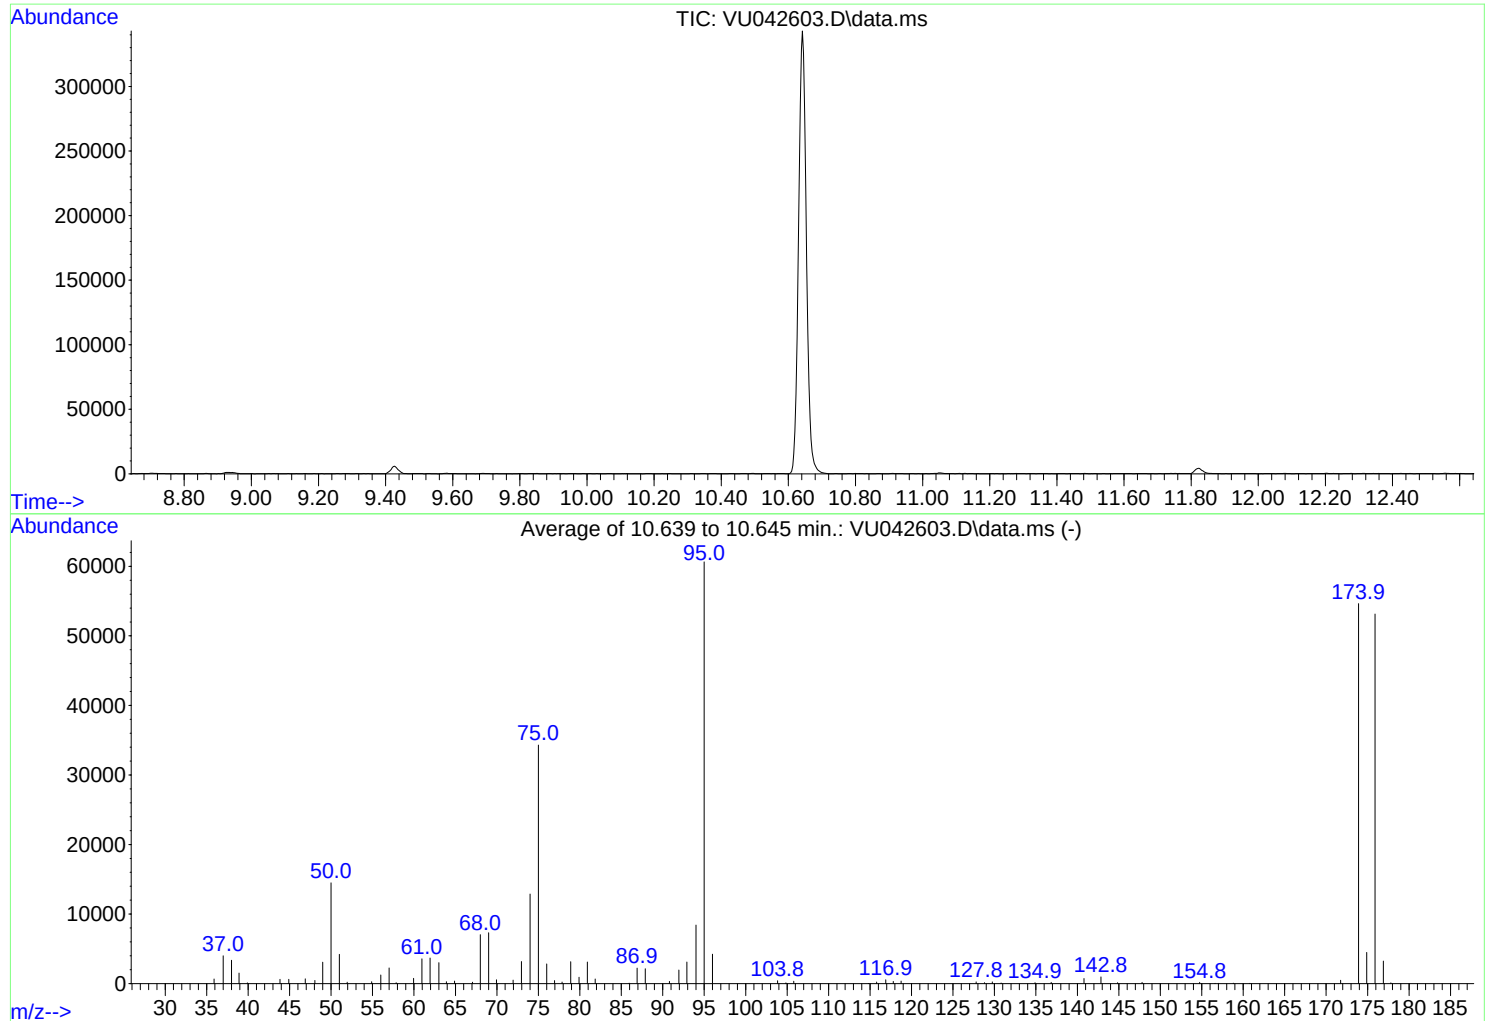

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	14488	PASS
75	95	30	80	56.5	34293	PASS
95	95	100	100	100.0	60643	PASS
96	95	5	9	7.0	4235	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.1	54645	PASS
175	174	5	9	8.2	4495	PASS
176	174	95	101	97.2	53136	PASS
177	176	5	9	6.1	3240	PASS

m/z	Abundance
35.90	636.0
37.00	3889.0
38.00	3439.0
38.90	1652.0
39.90	114.0
43.90	782.0
44.90	532.0
46.90	686.0
48.00	465.0
49.00	3071.0
50.00	14819.0
51.00	4124.0
51.90	185.0
54.90	273.0
56.00	1268.0
57.00	2221.0
57.80	120.0
59.90	631.0
61.00	3667.0
61.90	3563.0
63.00	3077.0
63.90	317.0
64.90	370.0
67.10	248.0
68.00	7265.0
69.00	7491.0
69.90	522.0
72.00	511.0
73.00	3155.0
74.00	13007.0
75.00	34432.0
76.00	2743.0
76.90	451.0
77.80	283.0
78.90	3252.0
79.90	922.0
80.90	3146.0
81.90	668.0
86.90	2297.0
87.90	2290.0
90.80	287.0
92.00	1897.0
92.90	3023.0
94.00	8196.0
95.00	59784.0
96.00	4167.0
103.90	438.0
104.90	126.0
105.80	309.0
115.80	228.0
116.90	577.0
117.80	319.0
118.80	327.0
127.80	251.0
128.80	158.0
129.70	242.0
130.80	140.0
134.90	127.0
136.80	190.0
140.80	779.0
142.90	918.0
144.80	153.0
147.80	188.0
154.80	158.0
156.60	132.0
158.80	114.0
171.70	450.0
173.90	52960.0
174.90	4578.0
175.90	51264.0
176.90	3264.0
177.80	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
35.90	708.0
37.00	4173.0
38.00	3465.0
38.90	1594.0
39.90	113.0
43.90	792.0
44.90	644.0
46.90	723.0
48.10	476.0
49.00	3207.0
50.00	14943.0
51.00	4294.0
51.90	214.0
54.90	311.0
56.00	1306.0
57.00	2336.0
57.80	153.0
60.00	755.0
60.90	3728.0
62.00	3836.0
63.00	3142.0
63.90	282.0
64.90	363.0
67.00	196.0
68.00	7271.0
69.00	7541.0
70.00	569.0
72.00	531.0
73.00	3255.0
74.00	13338.0
75.00	35384.0
76.00	2902.0
76.90	456.0
77.90	236.0
78.90	3278.0
79.90	951.0
80.90	3217.0
81.80	698.0
85.90	109.0
86.90	2296.0
87.90	2200.0
90.80	359.0
91.90	2014.0
92.90	3253.0
94.00	8690.0
95.00	62544.0
96.00	4415.0
103.80	445.0
104.90	135.0
105.80	355.0
115.80	243.0
116.90	589.0
117.80	348.0
118.70	366.0
127.80	257.0
128.80	152.0
129.80	268.0
130.80	119.0
134.90	148.0
136.90	196.0
140.80	740.0
142.80	1006.0
144.80	153.0
147.80	181.0
154.70	196.0
158.80	123.0
171.70	494.0
173.90	56192.0
174.90	4570.0
175.90	54952.0
176.90	3280.0
177.80	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
35.90	671.0
37.00	3920.0
38.00	3161.0
38.90	1342.0
39.90	100.0
43.90	725.0
44.90	682.0
46.90	651.0
48.10	435.0
49.00	3001.0
50.00	13701.0
51.00	4224.0
52.00	221.0
54.90	268.0
56.00	1167.0
57.00	2174.0
57.90	151.0
60.00	869.0
61.00	3316.0
62.00	3679.0
63.00	2848.0
63.90	243.0
64.90	346.0
67.00	150.0
68.00	6615.0
69.00	6912.0
70.00	602.0
71.90	476.0
72.90	3140.0
74.00	12306.0
75.00	33064.0
76.00	2815.0
77.00	383.0
77.90	181.0
78.90	2926.0
79.90	860.0
80.90	2970.0
81.80	667.0
86.00	110.0
86.90	2135.0
87.90	1949.0
90.80	345.0
91.90	1966.0
92.90	3026.0
94.00	8374.0
95.00	59600.0
96.00	4123.0
103.80	385.0
104.80	117.0
105.80	352.0
114.80	103.0
115.80	245.0
116.90	524.0
117.80	337.0
118.70	394.0
127.80	268.0
128.80	131.0
129.80	231.0
134.90	141.0
136.90	170.0
140.80	682.0
142.80	1000.0
144.90	137.0
147.80	175.0
154.70	177.0
157.00	109.0
160.80	117.0
171.80	478.0
173.90	54784.0
174.90	4338.0
175.90	53192.0
176.90	3175.0
177.80	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
43.80	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25