

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031419\
Data File : VU030006.D
Acq On : 12 Mar 2019 14:03
Operator : JC/SP
Sample : VU0314WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0314WBL01

Quant Time: Mar 13 06:41:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U031419DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Mar 13 04:21:52 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene	5.74	96	62414	1.00	ug/l	0.00

System Monitoring Compounds

57) 4-Bromofluorobenzene	10.31	95	20384	0.90	ug/l	0.00
Spiked Amount 1.000			Recovery	=	90.00%	
68) 1,2-Dichlorobenzene-d4	11.86	152	23696	0.92	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031419\
Data File : VU030006.D
Acq On : 12 Mar 2019 14:03
Operator : JC/SP
Sample : VU0314WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0314WBL01

Quant Time: Mar 13 06:41:04 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U031419DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Mar 13 04:21:52 2019
Response via : Initial Calibration

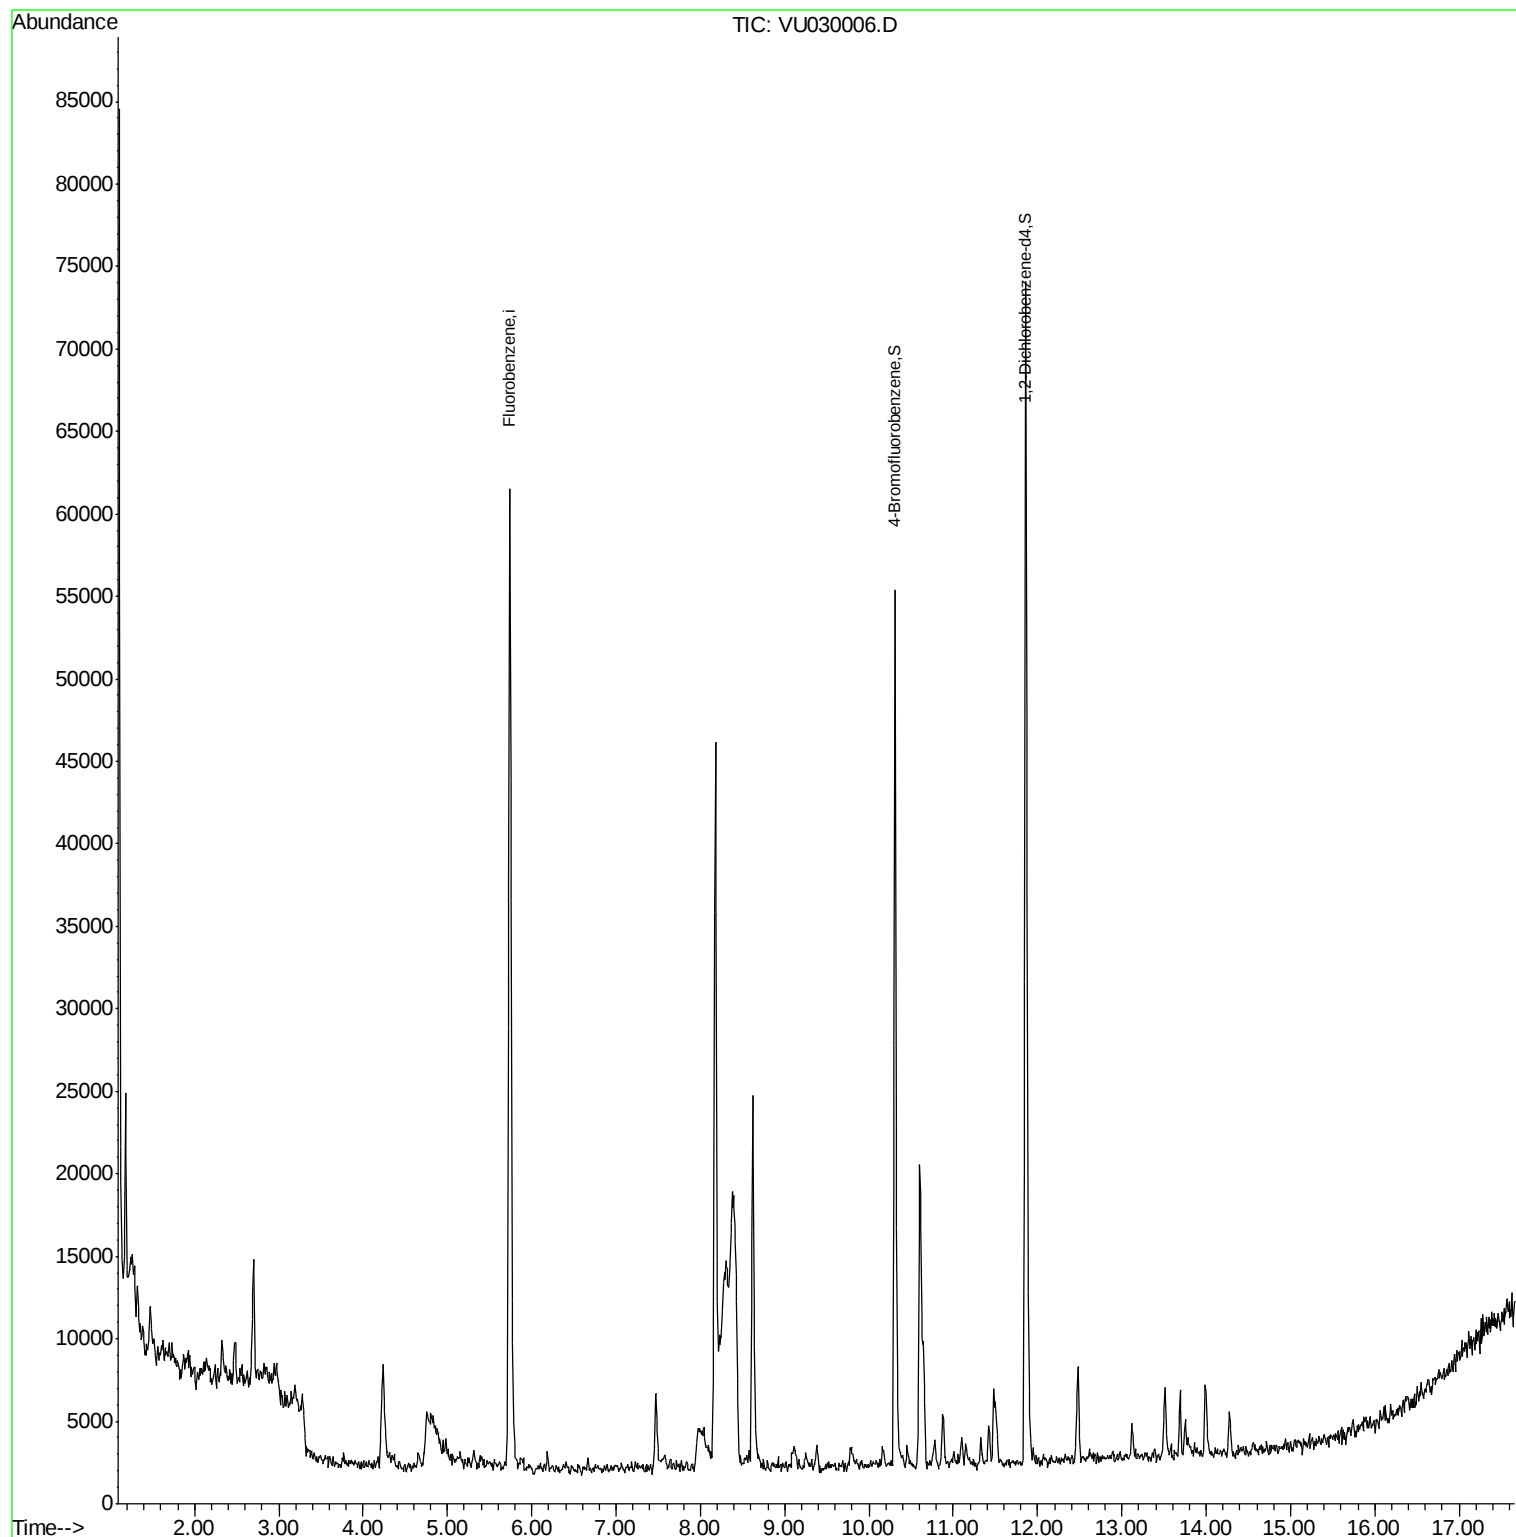

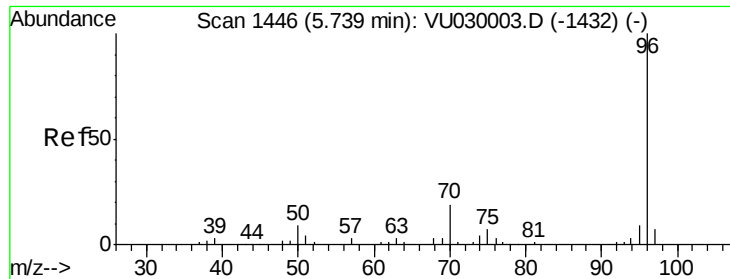

#1

Fluorobenzene

Concen: 1.000 ug/l

RT: 5.74 min Scan# 1446

Delta R.T. 0.00 min

Lab File: VU030006.D

Acq: 12 Mar 2019 14:03

Instrument :

MSVOA_U


ClientSampleId :

VU0314WBL01

Tgt Ion: 96 Resp: 62414

Ion Ratio Lower Upper

96	100		
70	19.8	15.5	23.3
95	8.8	6.6	9.8
97	6.7	0.0	0.0#



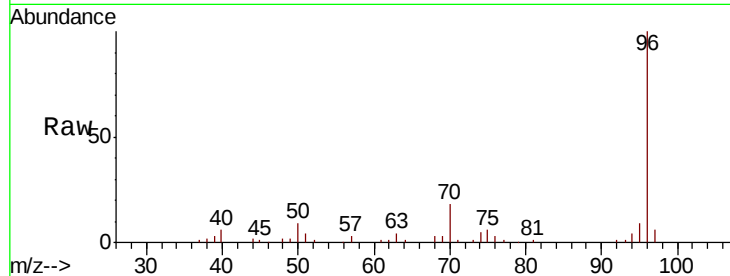


Abundance Ion 96.00 (95.70 to 96.70): VU0

Ion 70.00 (69.70 to 70.70): VU0

Ion 95.00 (94.70 to 95.70): VU0

Ion 97.00 (96.70 to 97.70): VU0

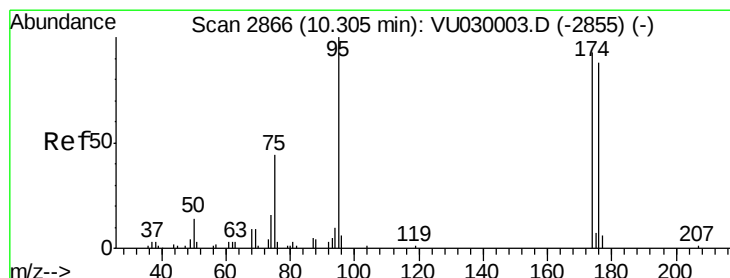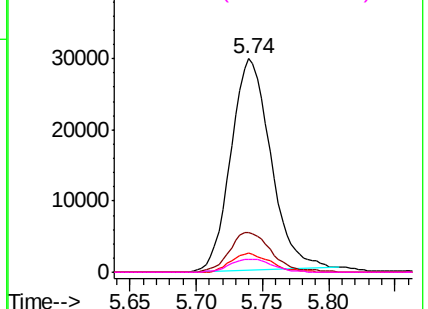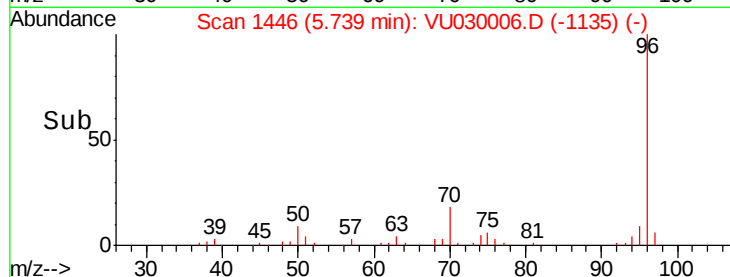

#57

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 10.31 min Scan# 2867

Delta R.T. 0.00 min


Lab File: VU030006.D

Acq: 12 Mar 2019 14:03

Tgt Ion: 95 Resp: 20384

Ion Ratio Lower Upper



95	100		
174	89.3	78.1	117.1
176	89.4	70.8	106.2

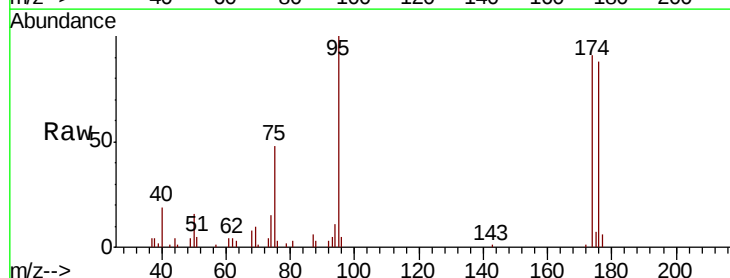


Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

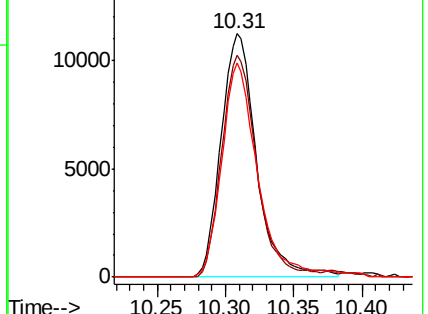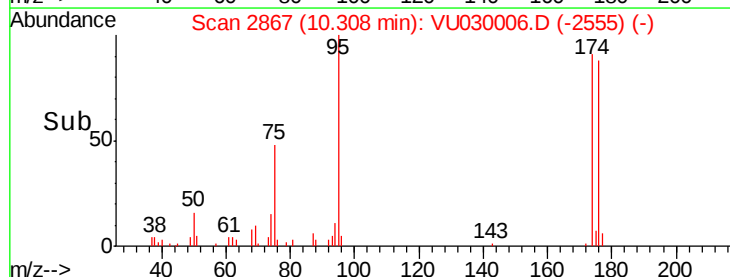


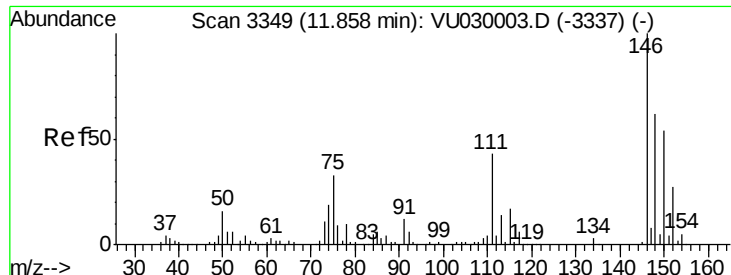

#68
 1,2-Dichlorobenzene-d4
 Concen: N.D. ug/l
 RT: 11.86 min Scan# 3349
 Delta R.T. 0.00 min
 Lab File: VU030006.D
 Acq: 12 Mar 2019 14:03

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0314WBL01

Tgt Ion	Ratio	Lower	Upper
152	100		
115	57.2	0.0	126.8
150	155.1	0.0	634.2

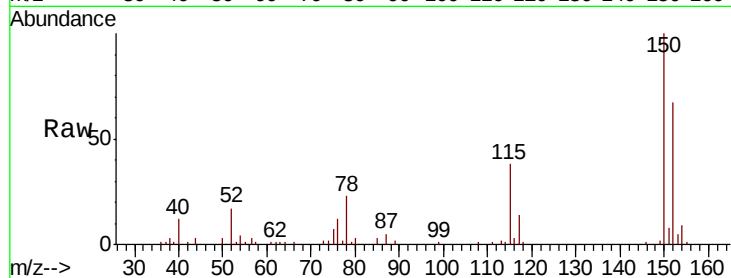

Abundance

Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

