

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031419\
 Data File : VU030007.D
 Acq On : 12 Mar 2019 14:37
 Operator : JC/SP
 Sample : K1850-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 38023-122017

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U031419DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.887	236	248	292	rVB	1791787	2679080	65.18%	7.278%
2	2.412	402	411	426	rVB	27202	49582	1.21%	0.135%
3	2.698	491	500	516	rVB2	25649	43950	1.07%	0.119%
4	3.000	575	594	640	rVB	1423488	3174061	77.22%	8.623%
5	3.437	713	730	750	rBV	203174	449002	10.92%	1.220%
6	4.219	950	973	1012	rBV	376770	1035073	25.18%	2.812%
7	4.543	1057	1074	1106	rBV2	282290	665422	16.19%	1.808%
8	5.129	1241	1256	1286	rBV	325563	721646	17.56%	1.960%
9	5.739	1430	1446	1471	rBV	60559	130896	3.18%	0.356%
10	6.556	1687	1700	1727	rBV	240758	472793	11.50%	1.284%
11	7.267	1909	1921	1944	rBV	192595	356030	8.66%	0.967%
12	7.878	2098	2111	2132	rBV	516214	894965	21.77%	2.431%
13	8.177	2191	2204	2213	rBV2	56848	110438	2.69%	0.300%
14	8.238	2213	2223	2245	rVV	369290	663499	16.14%	1.803%
15	9.206	2510	2524	2547	rBV	790220	1338365	32.56%	3.636%
16	10.164	2807	2822	2842	rBV	1262103	1942908	47.27%	5.278%
17	10.305	2856	2866	2881	rVB2	65258	103434	2.52%	0.281%
18	10.453	2899	2912	2918	rBV	558215	909285	22.12%	2.470%
19	10.492	2918	2924	2940	rVB	467640	738649	17.97%	2.007%
20	10.585	2940	2953	2968	rBV	1203204	1854745	45.12%	5.039%
21	10.768	2999	3010	3038	rVB	692639	1080112	26.28%	2.934%
22	11.144	3116	3127	3156	rVB	1535100	2321702	56.48%	6.307%
23	11.321	3166	3182	3198	rBV	1863918	2860645	69.59%	7.771%
24	11.414	3198	3211	3220	rVV	1591144	2493208	60.65%	6.773%
25	11.472	3220	3229	3259	rVB	2024181	3040123	73.96%	8.259%
26	11.887	3338	3358	3384	rBV	1021223	1665864	40.53%	4.526%
27	13.688	3905	3918	3933	rBV	2662019	4110540	100.00%	11.167%
28	13.983	3995	4010	4035	rBV	545944	903851	21.99%	2.455%


Sum of corrected areas: 36809868

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031419\
Data File : VU030007.D
Acq On : 12 Mar 2019 14:37
Operator : JC/SP
Sample : K1850-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
38023-122017

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U031419DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

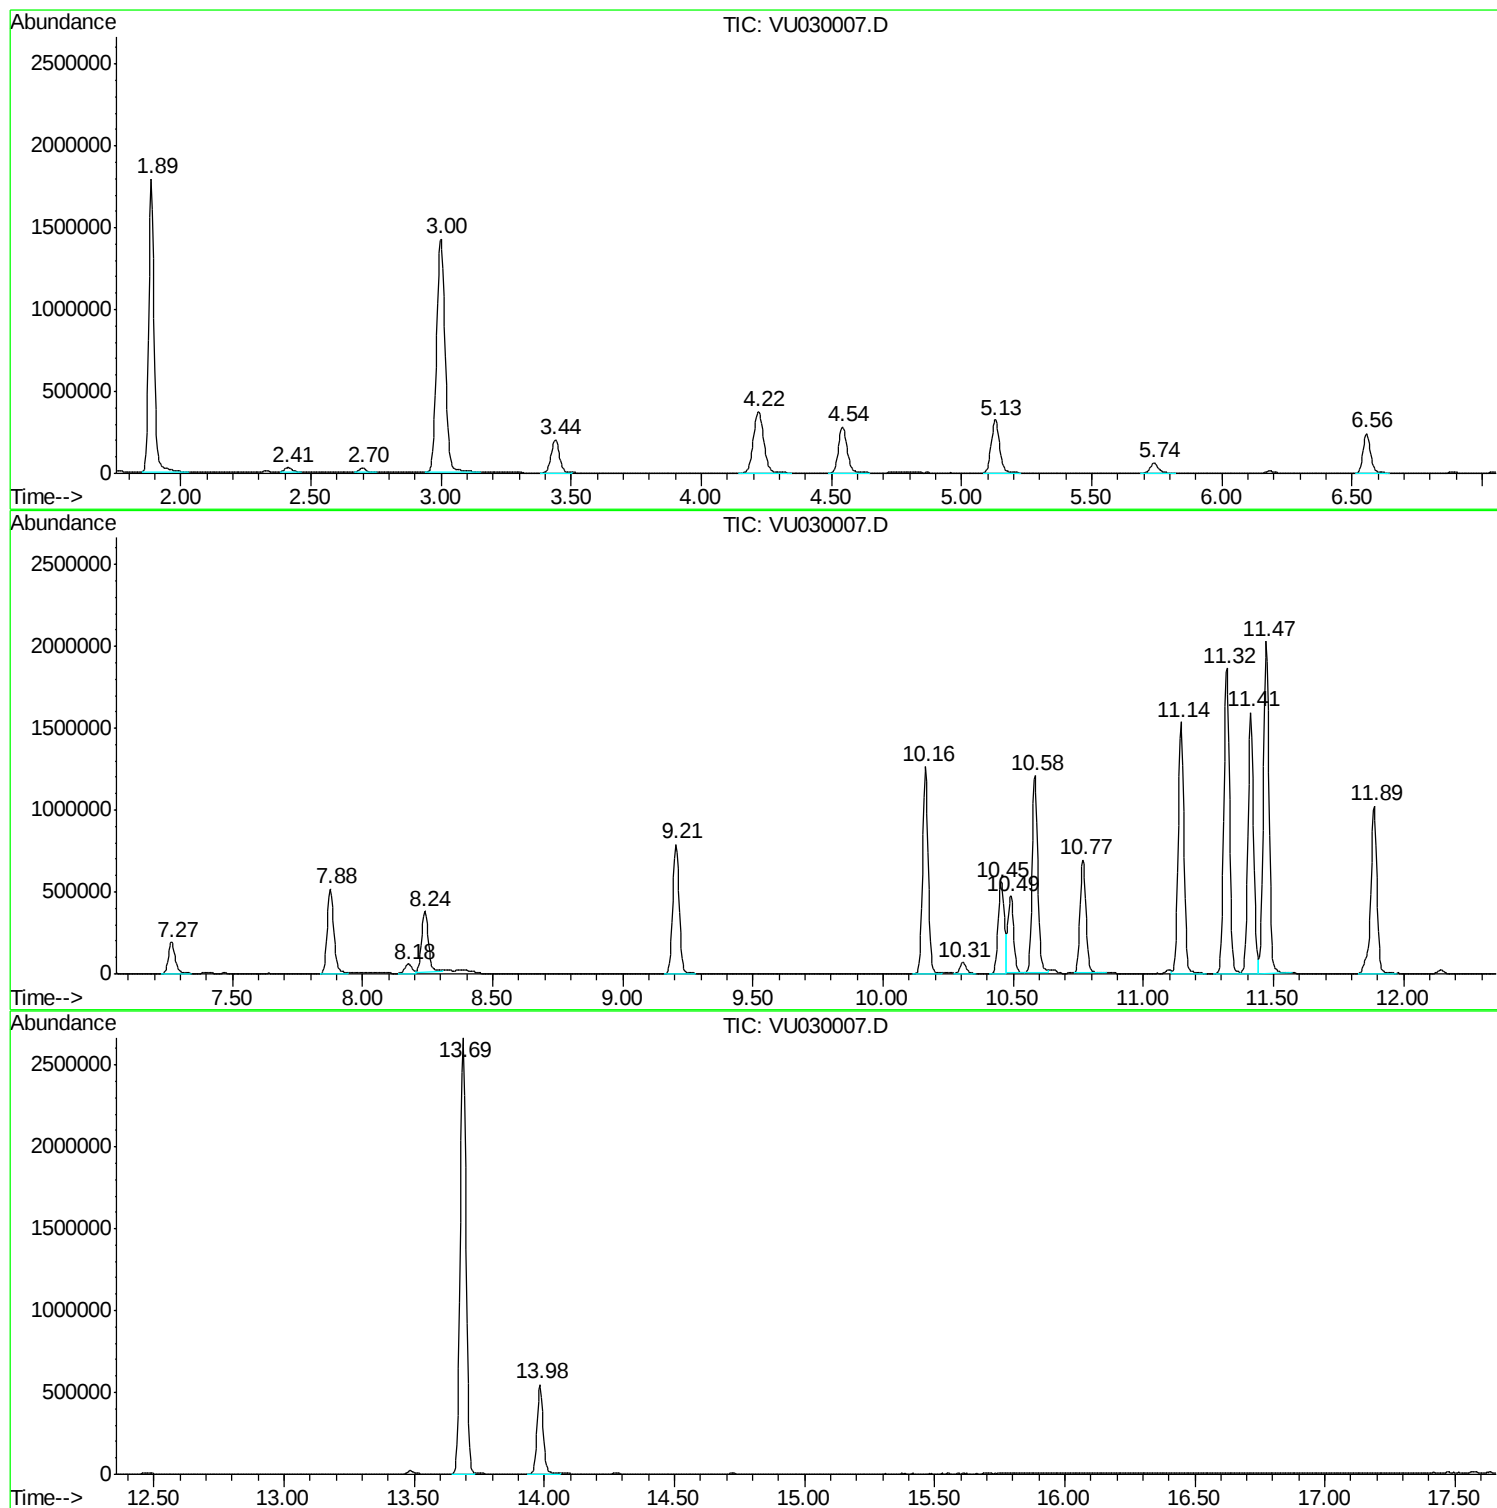

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031419\
Data File : VU030007.D
Acq On : 12 Mar 2019 14:37
Operator : JC/SP
Sample : K1850-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
38023-122017

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U031419DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031419\
Data File : VU030007.D
Acq On : 12 Mar 2019 14:37
Operator : JC/SP
Sample : K1850-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
38023-122017

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U031419DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc