


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031419\
 Data File : VU029998.D
 Acq On : 12 Mar 2019 08:47
 Operator : JC/SP
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U031419DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Wed Mar 13 04:21:52 2019

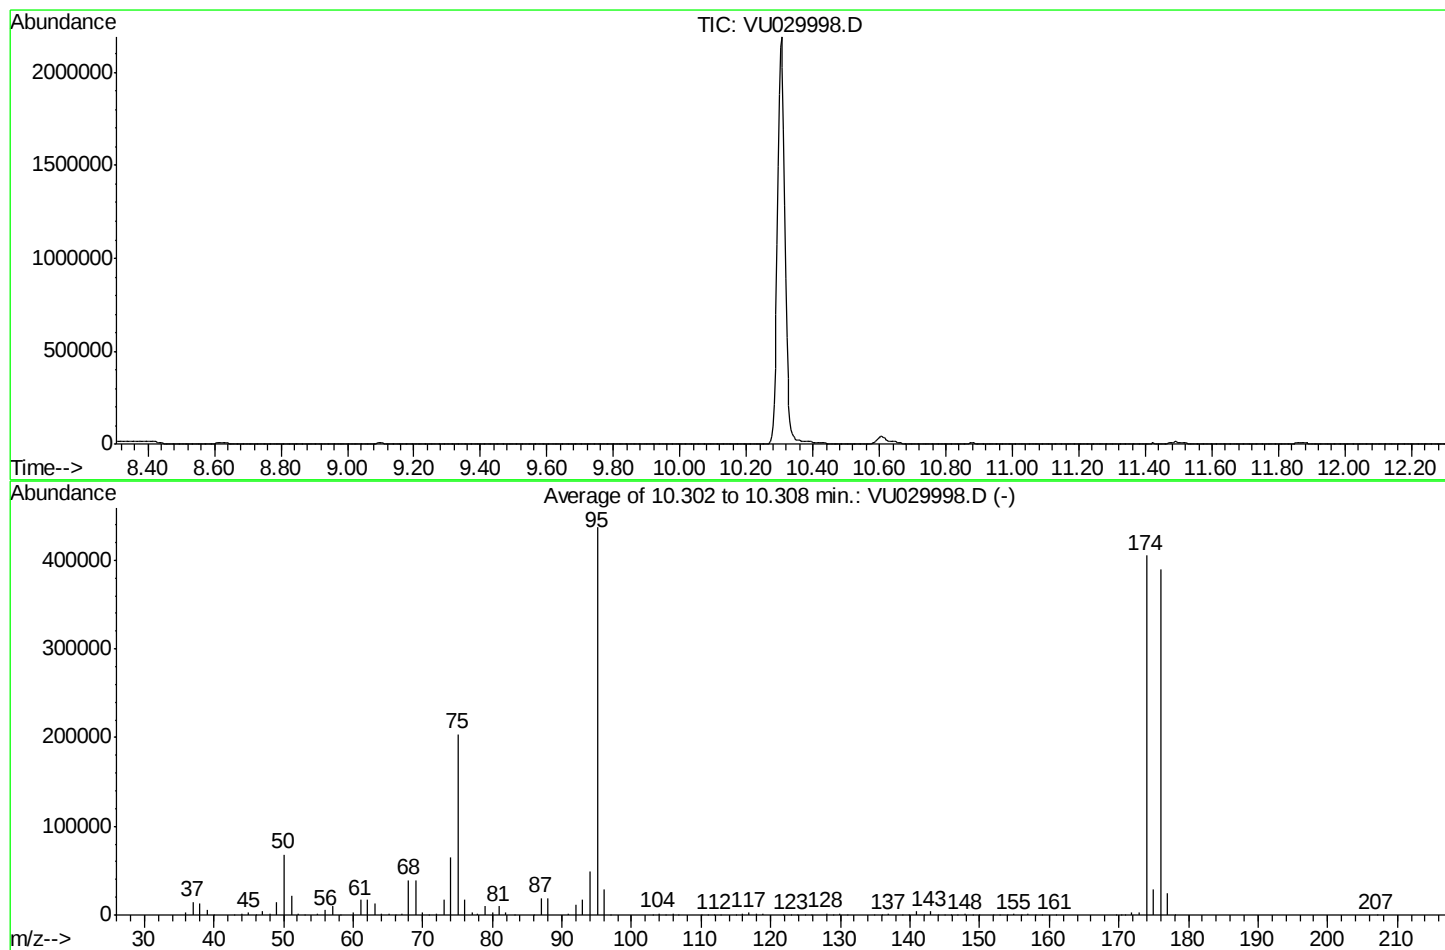

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	67840	PASS
75	95	30	60	46.6	203648	PASS
95	95	100	100	100.0	436970	PASS
96	95	5	9	6.8	29509	PASS
173	174	0.00	2	0.9	3532	PASS
174	95	50	100	92.7	405205	PASS
175	174	5	9	7.1	28621	PASS
176	174	95	101	96.3	390101	PASS
177	176	5	9	6.4	24789	PASS