

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031420\
 Data File : VU037265.D
 Acq On : 14 Mar 2020 16:09
 Operator : JC/MD
 Sample : L1900-17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0NE6

Quant Time: Mar 16 05:40:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 16 05:16:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	116903	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	116073	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	47755	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	34819	4.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.80%
7) Chloroethane-d5	1.93	69	31004	5.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	114.40%
11) 1,1-Dichloroethene-d2	2.59	63	49287	3.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.40%
20) 2-Butanone-d5	4.68	46	101821	51.85	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.70%
24) Chloroform-d	5.11	84	74744	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
26) 1,2-Dichloroethane-d4	5.74	65	45331	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.60%
32) Benzene-d6	5.76	84	132928	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.20%
36) 1,2-Dichloropropane-d6	6.72	67	43868	4.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.00%
41) Toluene-d8	7.93	98	121002	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.40%
43) trans-1,3-Dichloropropene-	8.21	79	16283	4.37	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.40%
46) 2-Hexanone-d5	8.66	63	79493	51.26	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.52%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	36215	4.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.40%
64) 1,2-Dichlorobenzene-d4	12.21	152	41504	5.03	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.60%


Target Compounds					Ovalue
13) Acetone	2.67	43	3448	2.143 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031420\
Data File : VU037265.D
Acq On : 14 Mar 2020 16:09
Operator : JC/MD
Sample : L1900-17
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NE6

Quant Time: Mar 16 05:40:14 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 16 05:16:55 2020
Response via : Initial Calibration

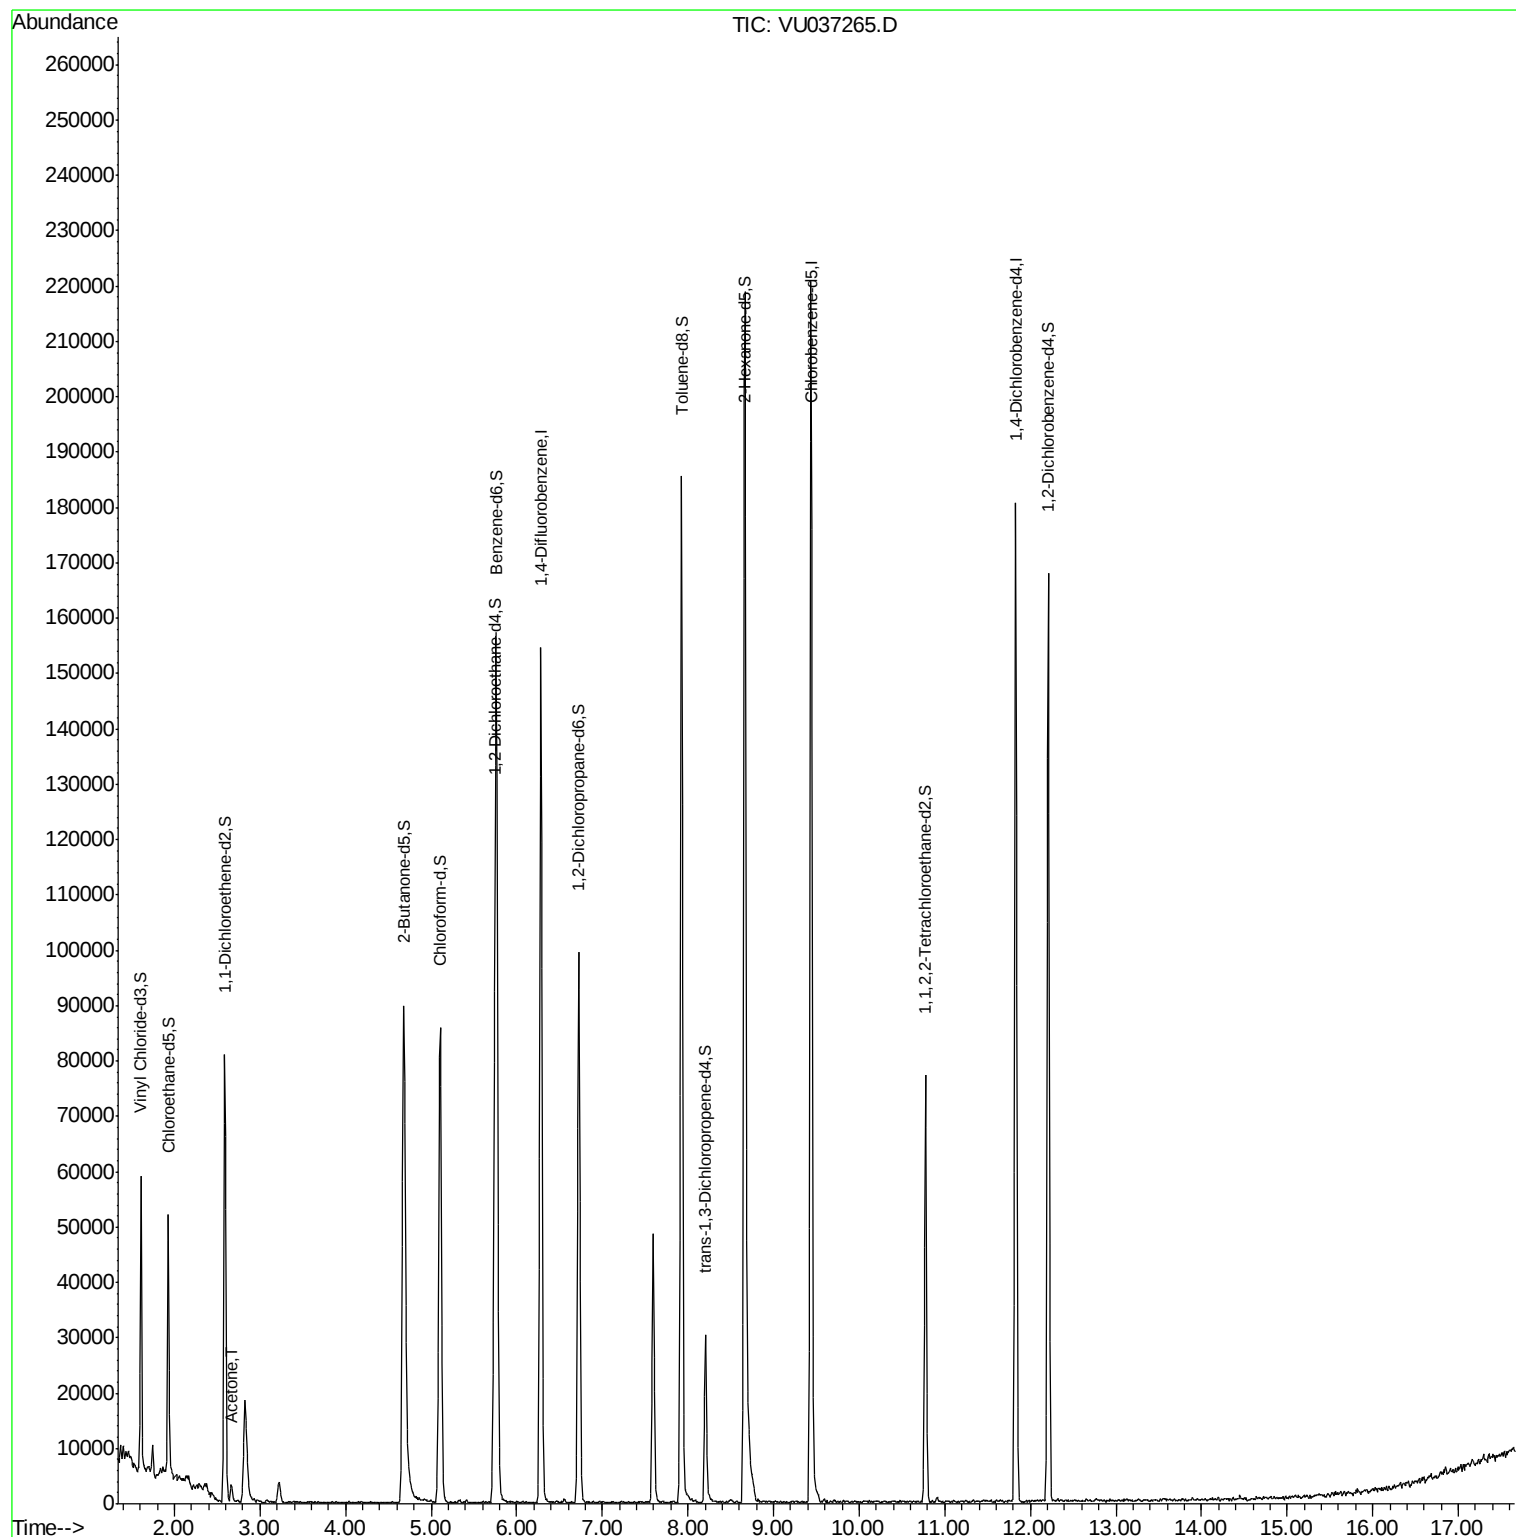

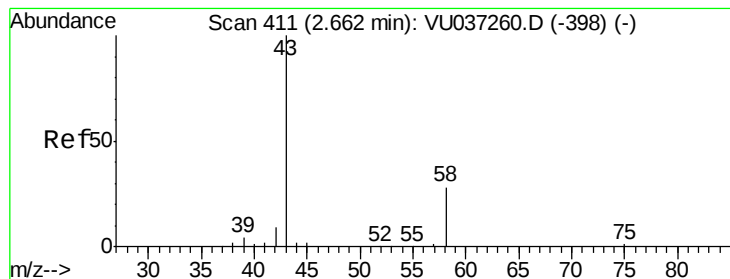

#13

Acetone

Concen: 2.143 ug/L

RT: 2.67 min Scan# 413

Delta R.T. 0.01 min

Lab File: VU037265.D

Acq: 14 Mar 2020 16:09

Instrument :

MSVOA_U

ClientSampleId :

CONE6

Tot Ion: 43 Resp: 3448

Ion Ratio Lower Upper

43 100

58 28.0 0.0 52.2

