

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031420\
 Data File : VU037269.D
 Acq On : 14 Mar 2020 17:48
 Operator : JC/MD
 Sample : L1923-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CONGO

Quant Time: Mar 16 05:58:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 16 05:16:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	117465	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	120865	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	49336	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	36071	4.68	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.60%
7) Chloroethane-d5	1.93	69	31746	5.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.60%
11) 1,1-Dichloroethene-d2	2.59	63	52000	3.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.40%
20) 2-Butanone-d5	4.67	46	100812	51.10	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.20%
24) Chloroform-d	5.11	84	74252	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	5.74	65	46558	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
32) Benzene-d6	5.76	84	137769	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
36) 1,2-Dichloropropane-d6	6.72	67	43968	4.58	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.60%
41) Toluene-d8	7.93	98	123545	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
43) trans-1,3-Dichloropropene-	8.21	79	17006	4.39	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.80%
46) 2-Hexanone-d5	8.66	63	77739	48.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.28%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	36961	4.68	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.60%
64) 1,2-Dichlorobenzene-d4	12.21	152	44764	5.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.00%


Target Compounds					Ovalue
13) Acetone	2.66	43	4726	2.923 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031420\
Data File : VU037269.D
Acq On : 14 Mar 2020 17:48
Operator : JC/MD
Sample : L1923-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0NG0

Quant Time: Mar 16 05:58:25 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 16 05:16:55 2020
Response via : Initial Calibration

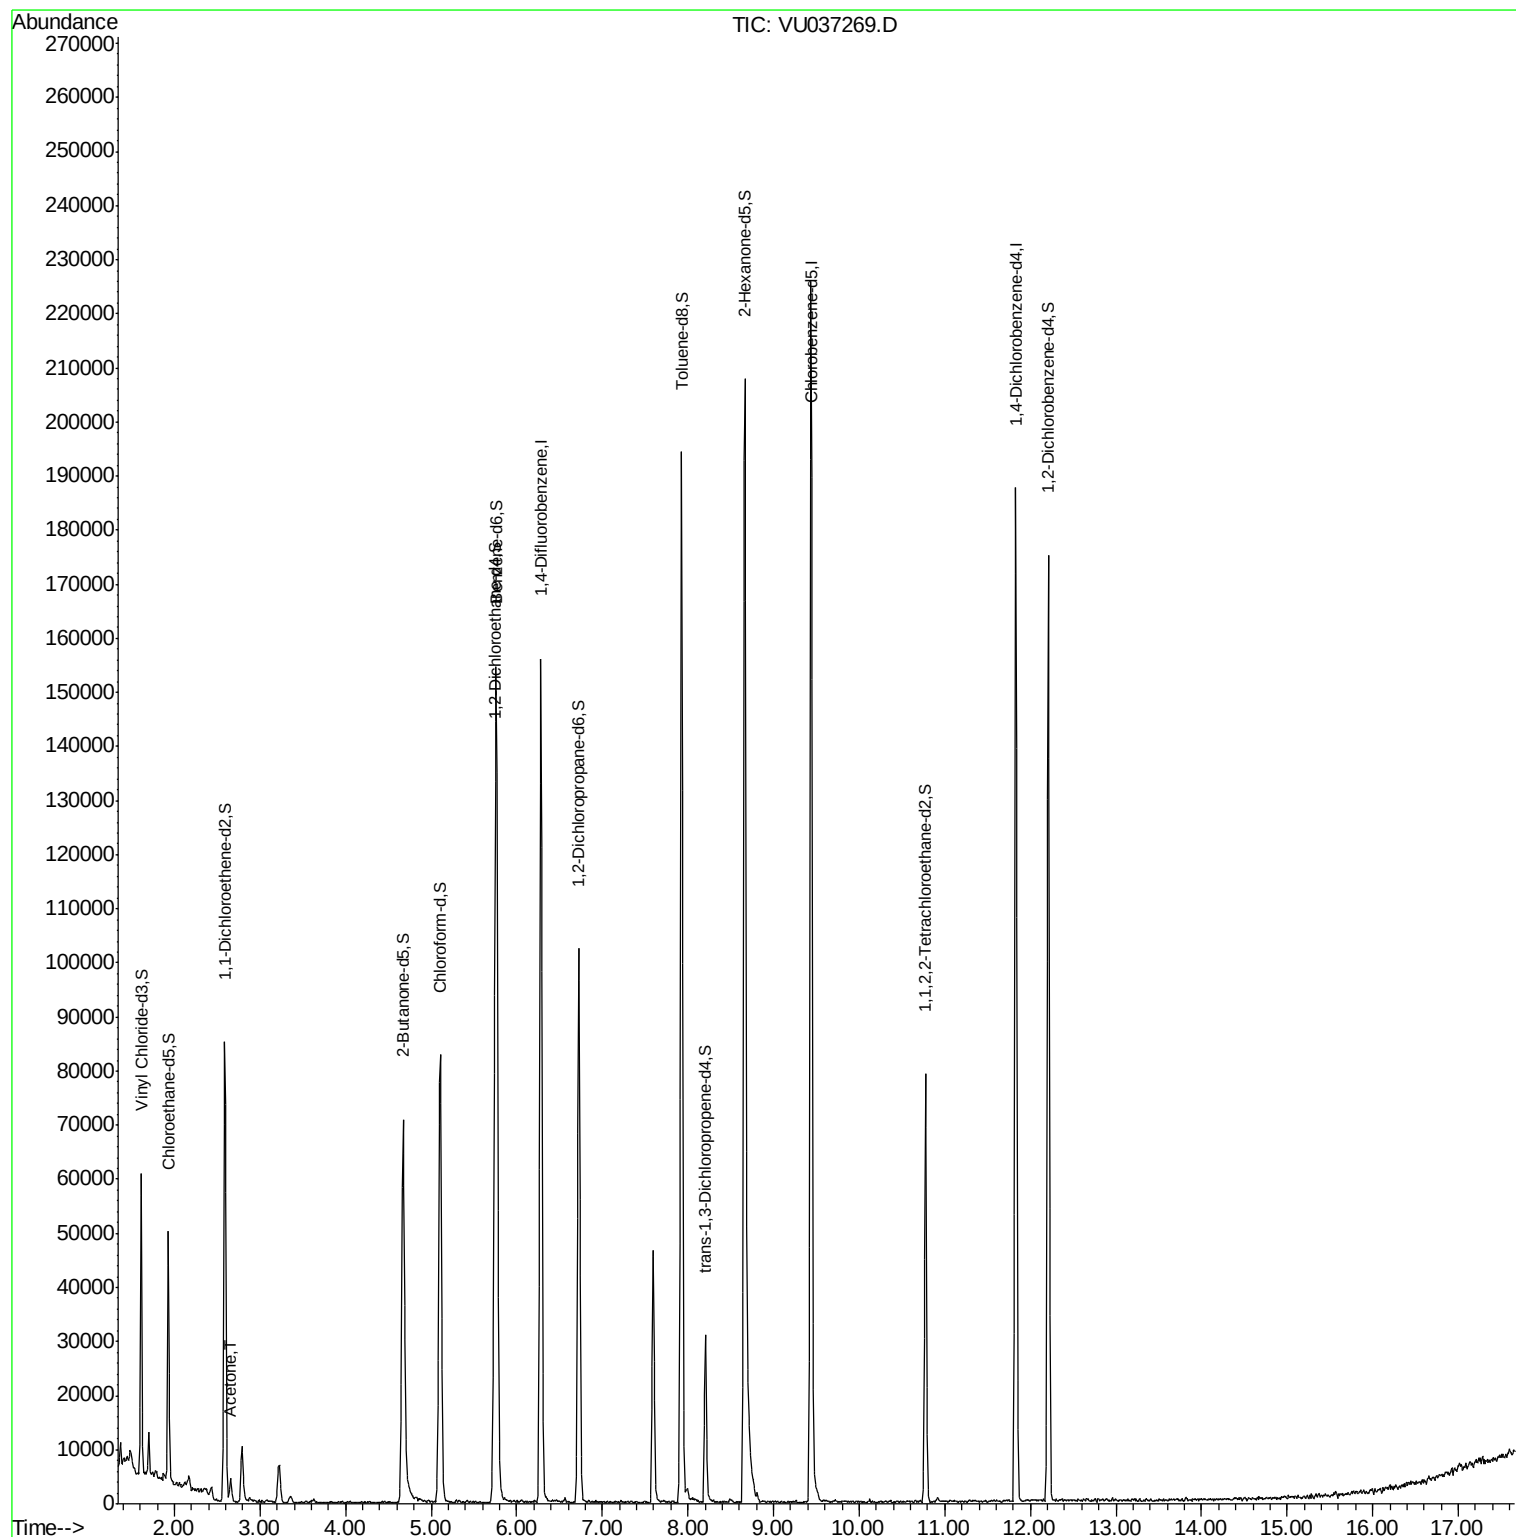

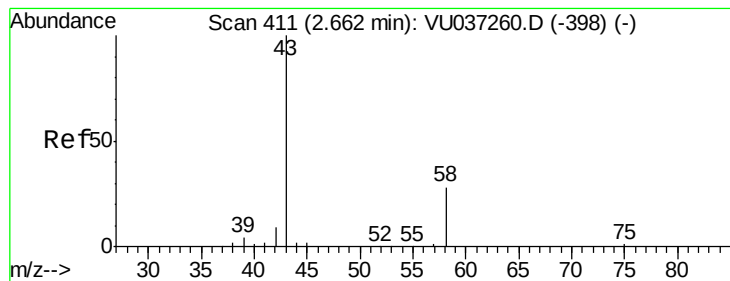

#13
 Acetone
 Concen: 2.923 ug/L
 RT: 2.66 min Scan# 410
 Delta R.T. -0.00 min
 Lab File: VU037269.D
 Acq: 14 Mar 2020 17:48

Instrument :
 MSVOA_U
 ClientSampleId :
 CONGO

Tot Ion: 43 Resp: 4726
 Ion Ratio Lower Upper
 43 100
 58 29.4 0.0 52.2

