

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031420\
 Data File : VU037278.D
 Acq On : 14 Mar 2020 21:31
 Operator : JC/MD
 Sample : L1923-13
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CONJO

Quant Time: Mar 16 06:55:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 16 05:16:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	119952	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	117136	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	48005	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	35536	4.51	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.20%
7) Chloroethane-d5	1.93	69	31057	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.60%
11) 1,1-Dichloroethene-d2	2.59	63	51694	3.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.60%
20) 2-Butanone-d5	4.67	46	99395	49.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.66%
24) Chloroform-d	5.10	84	76650	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
26) 1,2-Dichloroethane-d4	5.74	65	45365	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.00%
32) Benzene-d6	5.76	84	136976	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.20%
36) 1,2-Dichloropropane-d6	6.73	67	44161	4.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.80%
41) Toluene-d8	7.93	98	124450	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
43) trans-1,3-Dichloropropene-	8.21	79	16362	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.66	63	75001	47.92	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.84%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	36812	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.20%
64) 1,2-Dichlorobenzene-d4	12.21	152	43037	5.19	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.80%


Target Compounds					Ovalue
13) Acetone	2.66	43	1865	1.130 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU031420\
Data File : VU037278.D
Acq On : 14 Mar 2020 21:31
Operator : JC/MD
Sample : L1923-13
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONJO

Quant Time: Mar 16 06:55:51 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 16 05:16:55 2020
Response via : Initial Calibration

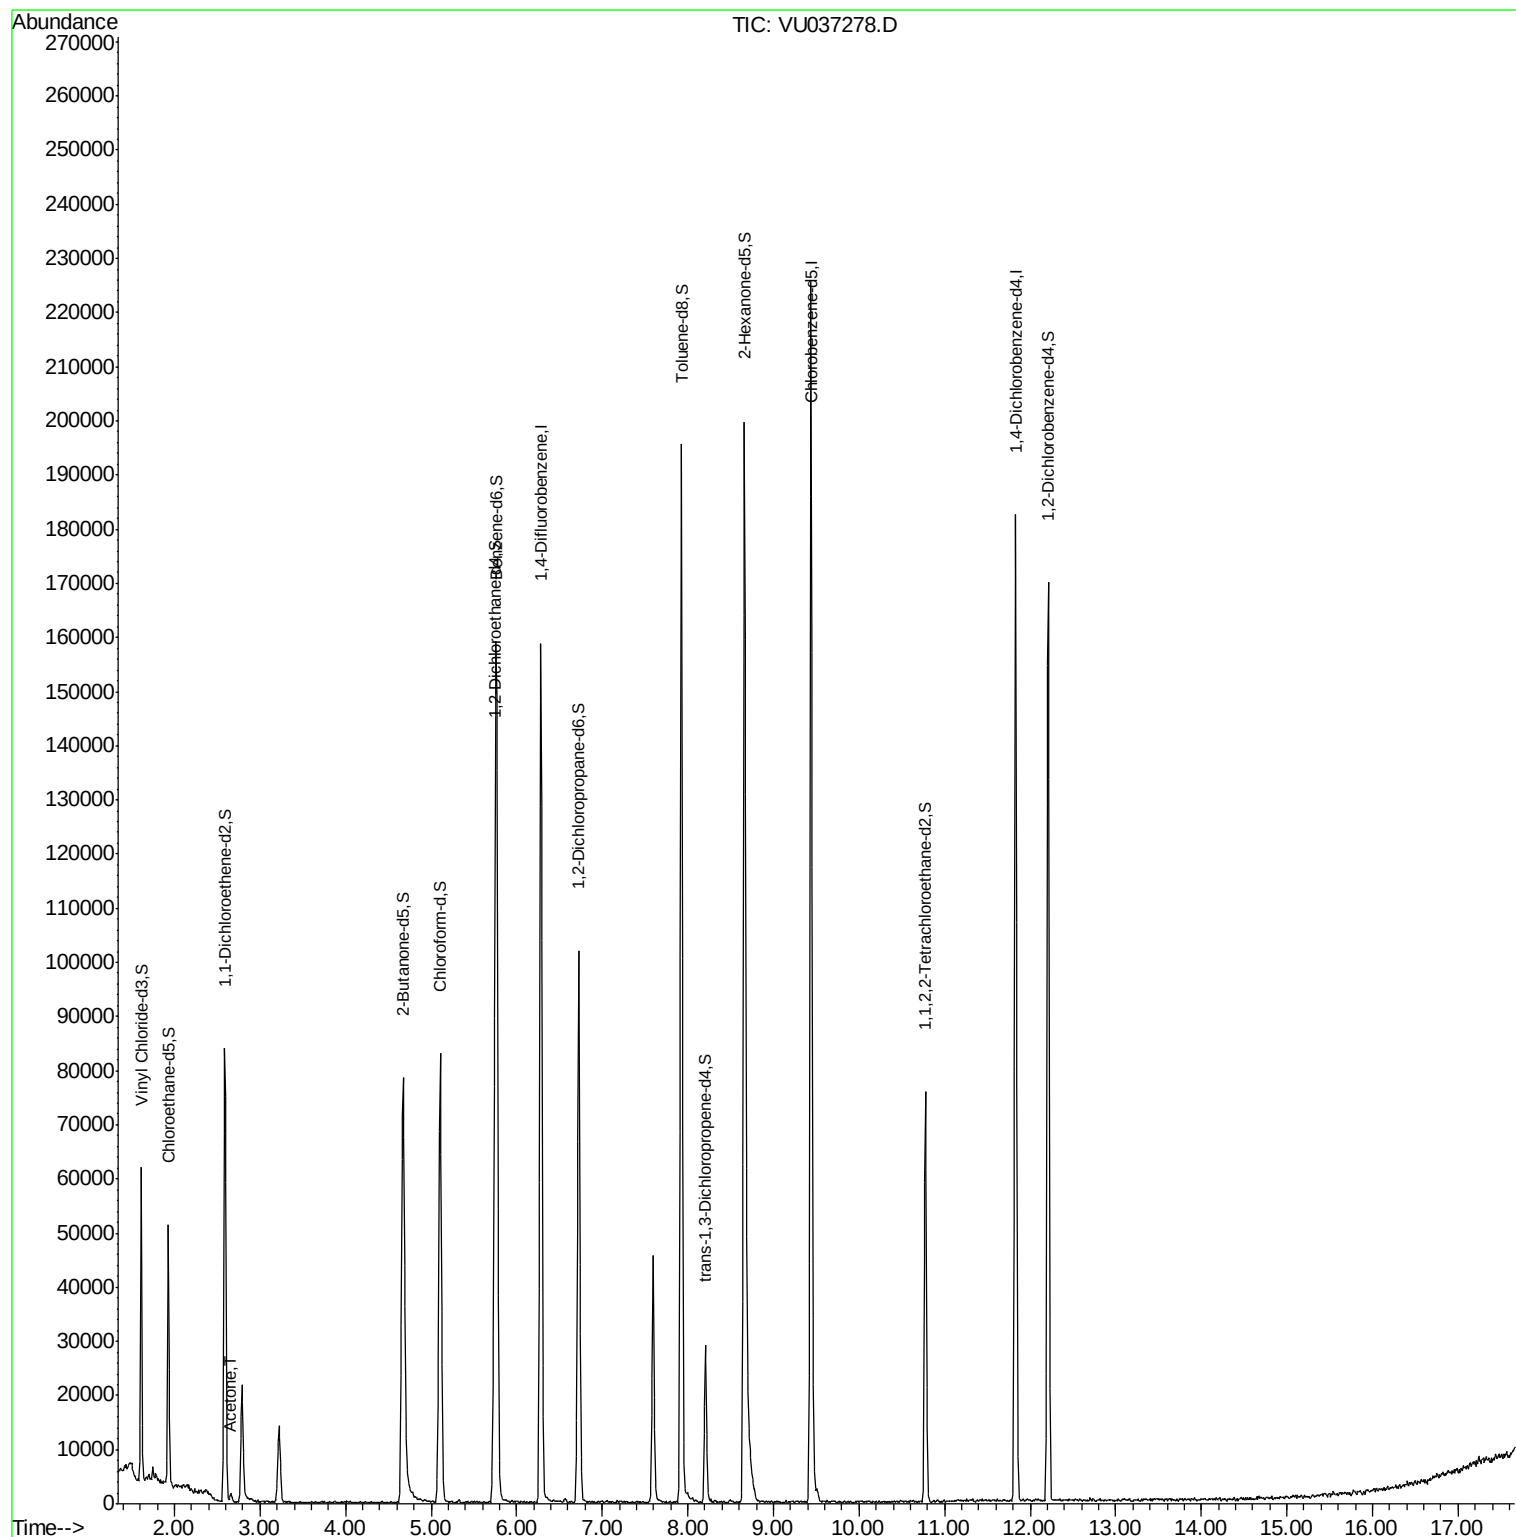

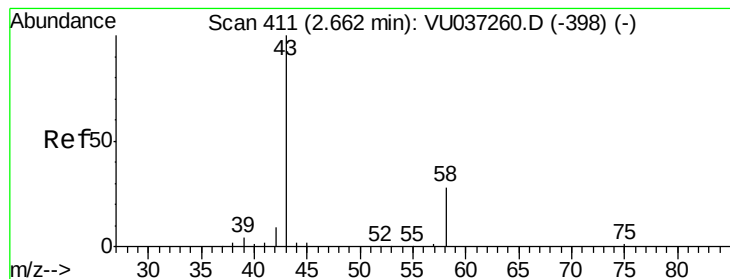

#13
 Acetone
 Concen: 1.130 ug/L
 RT: 2.66 min Scan# 411
 Delta R.T. 0.00 min
 Lab File: VU037278.D
 Acq: 14 Mar 2020 21:31

Instrument :
 MSVOA_U
 ClientSampleId :
 CONJO

Tot Ion: 43 Resp: 1865
 Ion Ratio Lower Upper
 43 100
 58 28.4 0.0 52.2

