

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031420\
 Data File : VU037279.D
 Acq On : 14 Mar 2020 21:56
 Operator : JC/MD
 Sample : L1923-14
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CONJ3

Quant Time: Mar 16 06:58:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 16 05:16:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	122461	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	122886	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	49161	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	34957	4.35	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.00%
7) Chloroethane-d5	1.93	69	31305	5.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.20%
11) 1,1-Dichloroethene-d2	2.59	63	50462	3.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.80%
20) 2-Butanone-d5	4.67	46	96719	47.02	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.04%
24) Chloroform-d	5.11	84	74710	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
26) 1,2-Dichloroethane-d4	5.74	65	44527	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.40%
32) Benzene-d6	5.76	84	136660	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
36) 1,2-Dichloropropane-d6	6.72	67	45126	4.62	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.40%
41) Toluene-d8	7.93	98	120039	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.80%
43) trans-1,3-Dichloropropene-	8.21	79	16645	4.22	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.40%
46) 2-Hexanone-d5	8.66	63	76830	46.79	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.58%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	35929	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.40%
64) 1,2-Dichlorobenzene-d4	12.21	152	43880	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
13) Acetone	2.66	43	2012	1.194 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031420\
Data File : VU037279.D
Acq On : 14 Mar 2020 21:56
Operator : JC/MD
Sample : L1923-14
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONJ3

Quant Time: Mar 16 06:58:50 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 16 05:16:55 2020
Response via : Initial Calibration

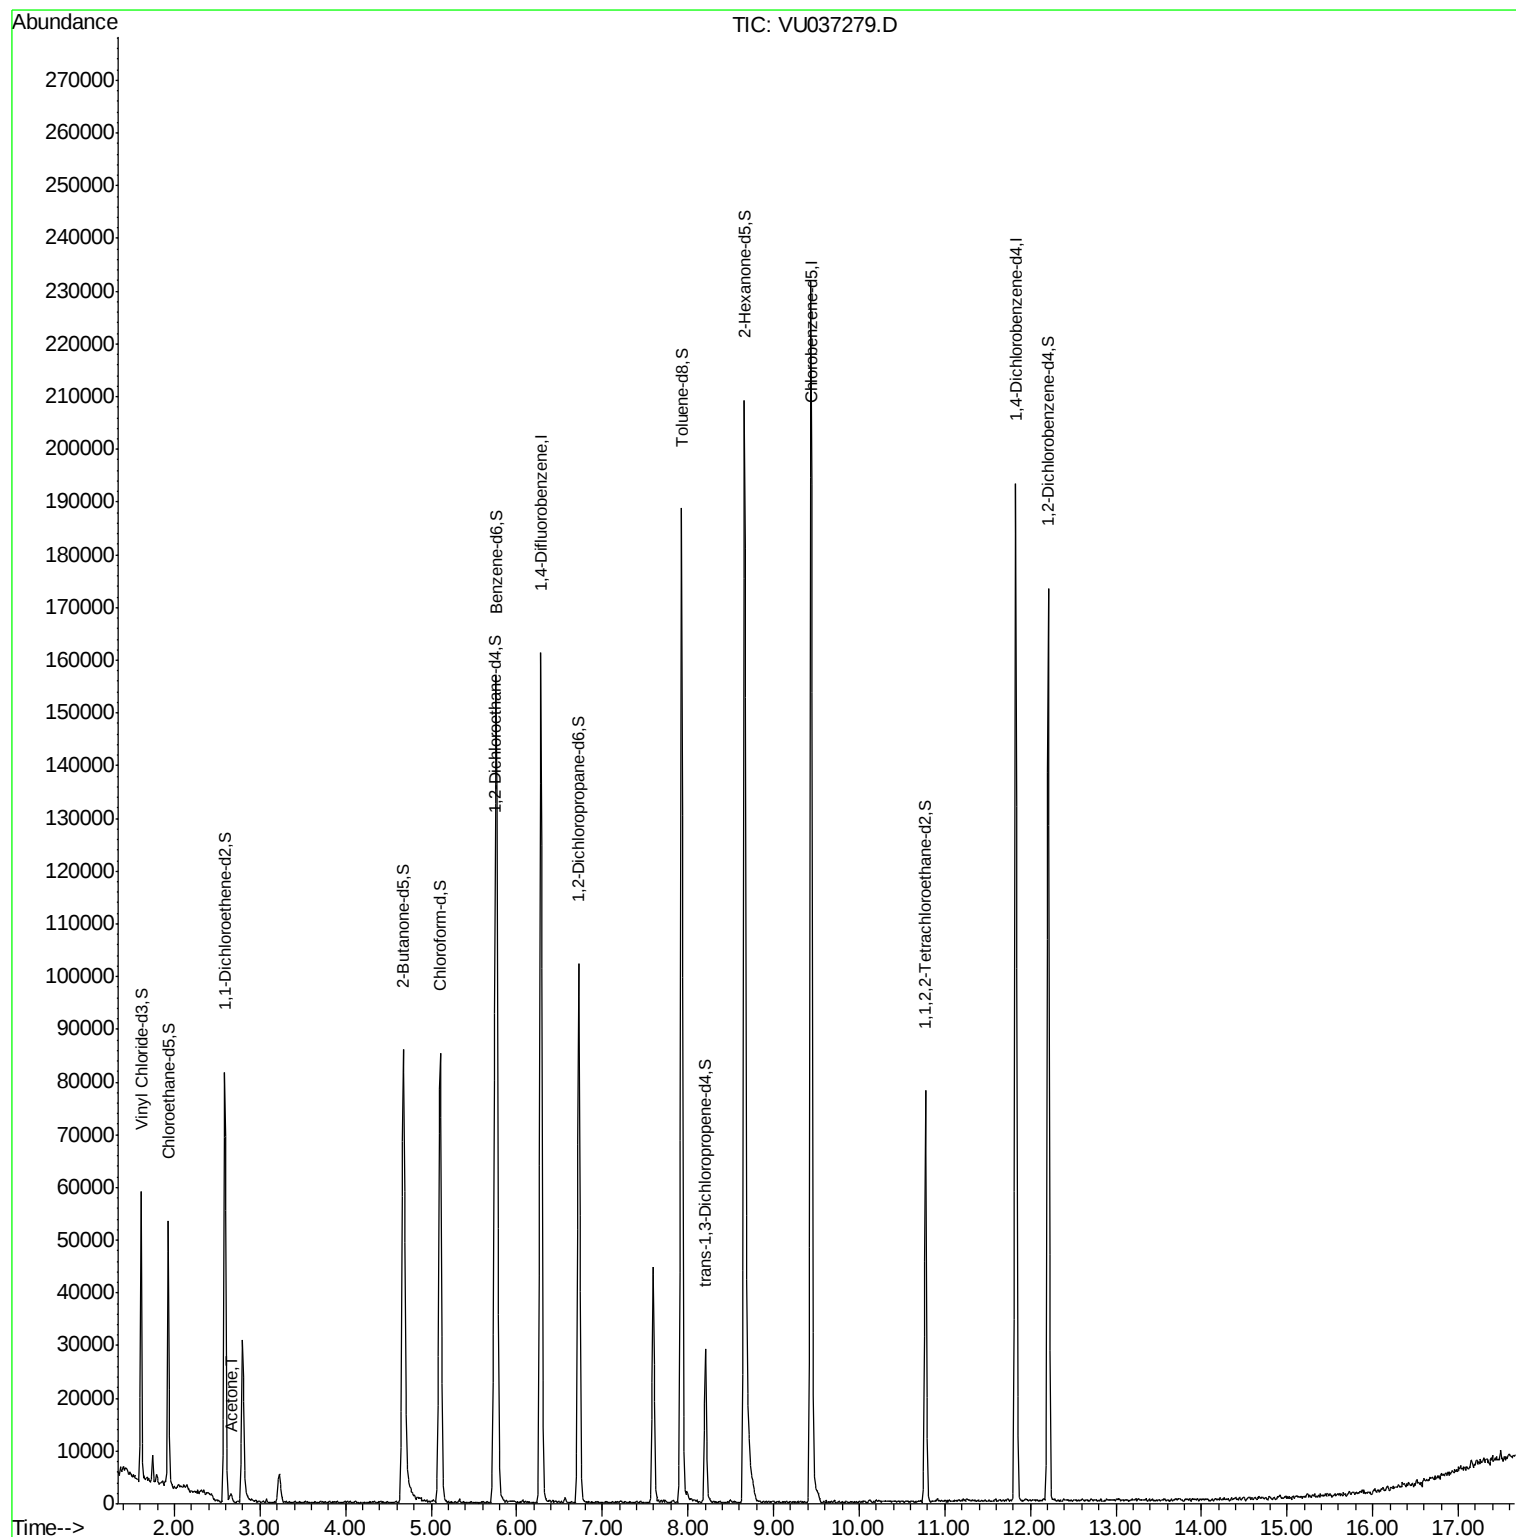

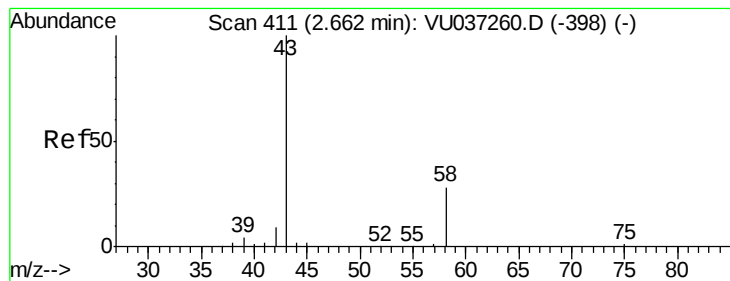

#13
 Acetone
 Concen: 1.194 ug/L
 RT: 2.66 min Scan# 411
 Delta R.T. 0.00 min
 Lab File: VU037279.D
 Acq: 14 Mar 2020 21:56

Instrument :
 MSVOA_U
 ClientSampleId :
 CONJ3

Tot Ion: 43 Resp: 2012
 Ion Ratio Lower Upper
 43 100
 58 22.3 0.0 52.2

