

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031420\
 Data File : VU037282.D
 Acq On : 14 Mar 2020 23:10
 Operator : JC/MD
 Sample : L1923-17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 CONJ8

Quant Time: Mar 16 07:07:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Mar 16 05:16:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	121846	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	122368	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	49432	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	35509	4.44	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.80%
7) Chloroethane-d5	1.93	69	31051	5.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.80%
11) 1,1-Dichloroethene-d2	2.59	63	50438	3.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.20%
20) 2-Butanone-d5	4.67	46	95710	46.77	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.54%
24) Chloroform-d	5.11	84	76665	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
26) 1,2-Dichloroethane-d4	5.74	65	45173	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	5.76	84	136638	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
36) 1,2-Dichloropropane-d6	6.73	67	44509	4.57	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.40%
41) Toluene-d8	7.92	98	120284	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.40%
43) trans-1,3-Dichloropropene-	8.20	79	16367	4.17	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.40%
46) 2-Hexanone-d5	8.66	63	73365	44.87	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.74%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	36297	4.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.80%
64) 1,2-Dichlorobenzene-d4	12.21	152	44019	5.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.20%


Target Compounds					Ovalue
13) Acetone	2.65	43	3040	1.813 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU031420\
Data File : VU037282.D
Acq On : 14 Mar 2020 23:10
Operator : JC/MD
Sample : L1923-17
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
CONJ8

Quant Time: Mar 16 07:07:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Mar 16 05:16:55 2020
Response via : Initial Calibration

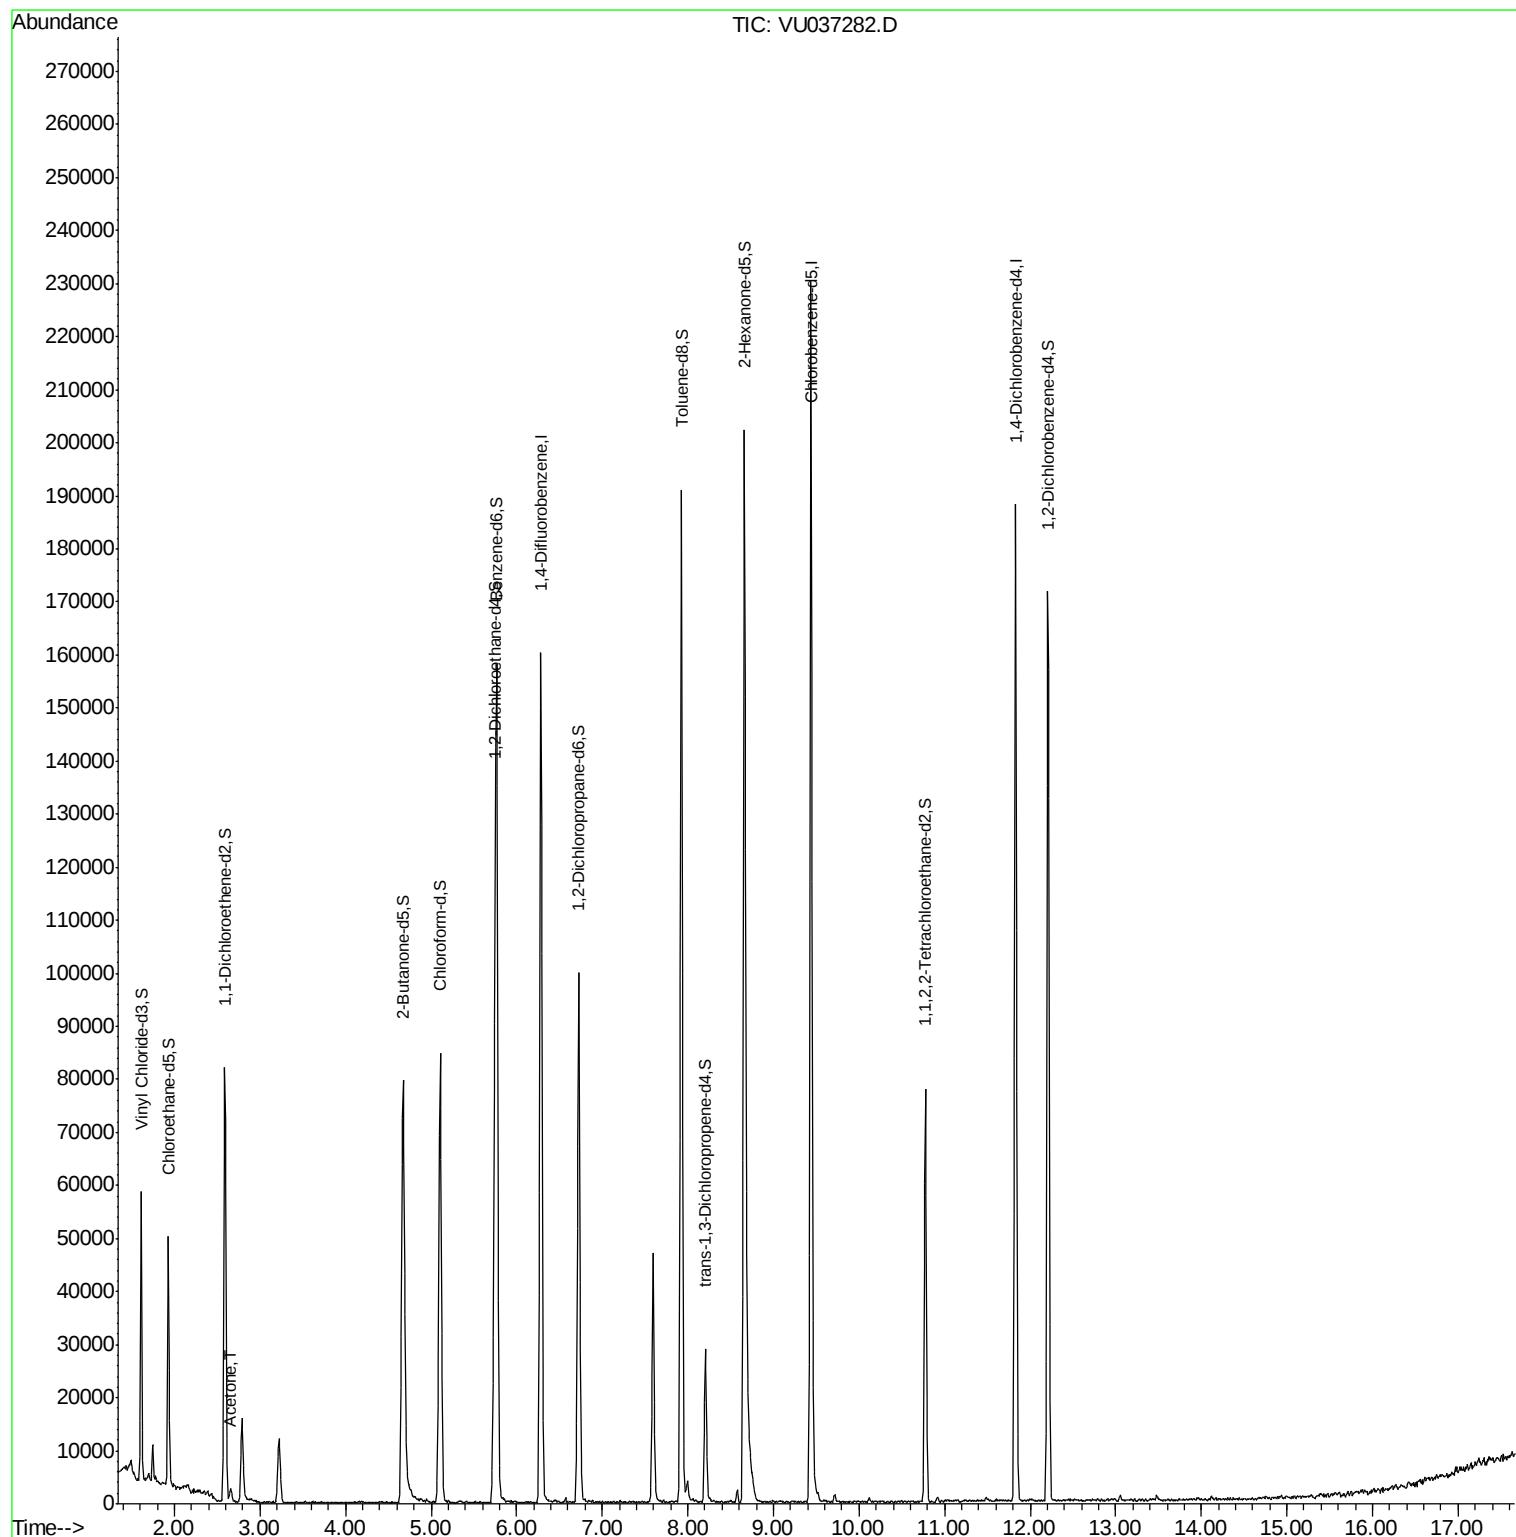

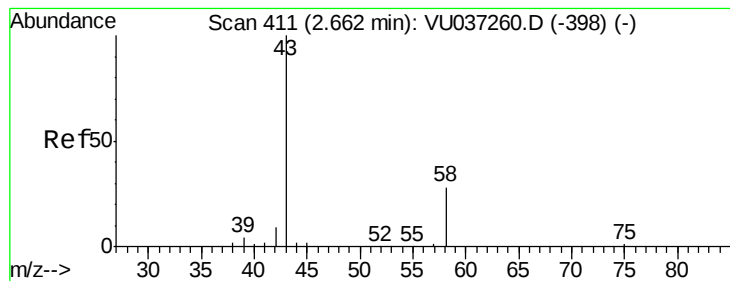

#13

Acetone

Concen: 1.813 ug/L

RT: 2.65 min Scan# 409

Delta R.T. -0.01 min

Lab File: VU037282.D

Acq: 14 Mar 2020 23:10

Instrument :
MSVOA_U
ClientSampleId :
CONJ8

Tot Ion: 43 Resp: 3040

Ion Ratio Lower Upper

43 100

58 29.9 0.0 52.2

