


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU031420\
 Data File : VU037259.D
 Acq On : 14 Mar 2020 12:55
 Operator : JC/MD
 Sample : BFB04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR031120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Mar 16 17:39:13 2020

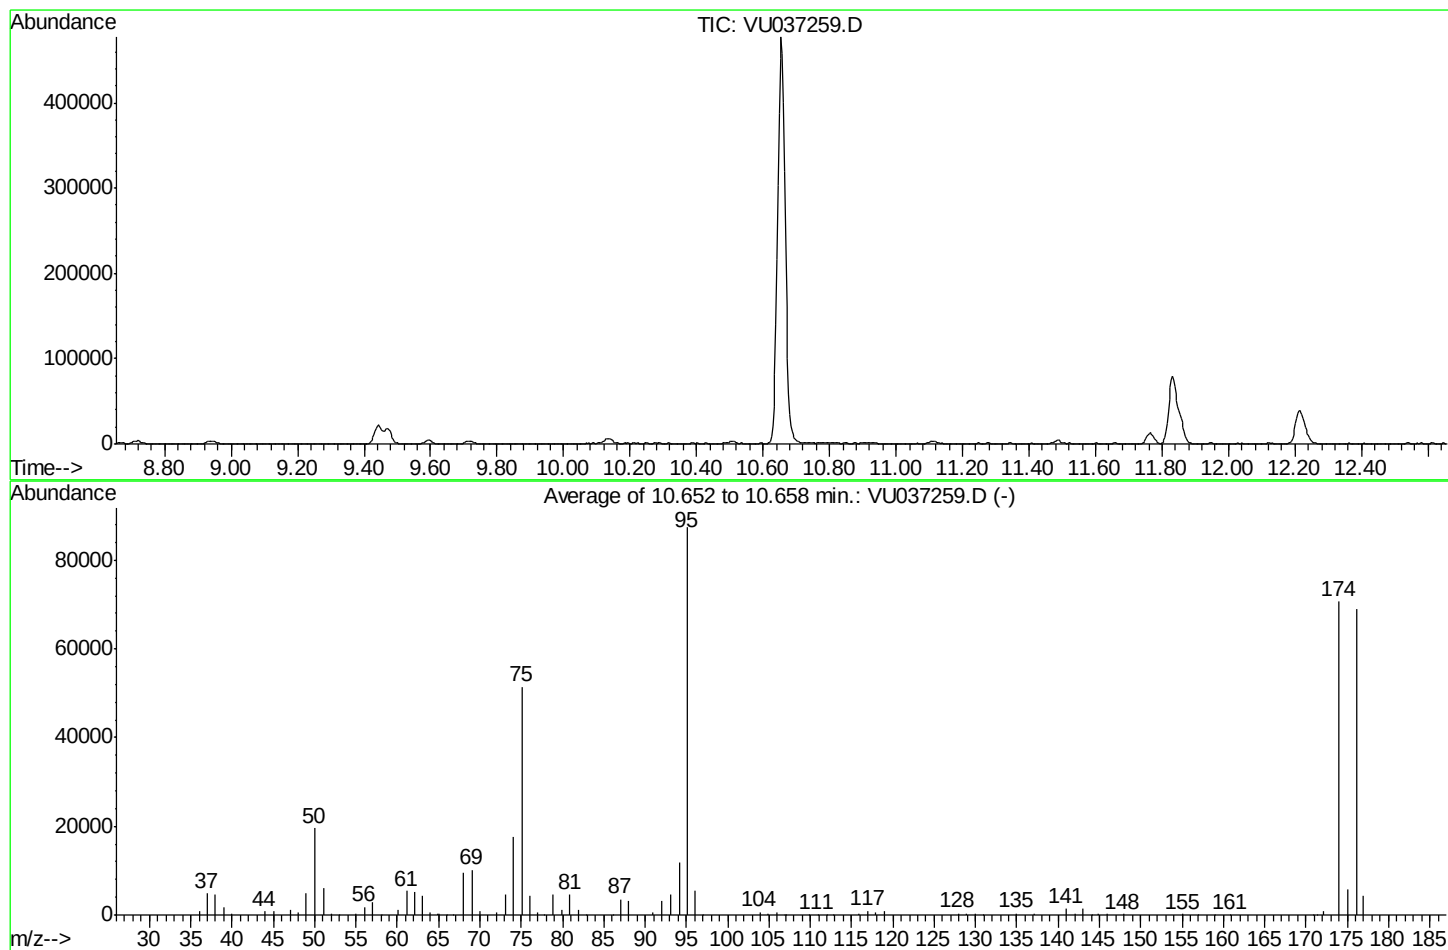

AutoFind: Scans 2896, 2897, 2898; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	19552	PASS
75	95	30	80	58.9	51517	PASS
95	95	100	100	100.0	87405	PASS
96	95	5	9	6.4	5637	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.8	70637	PASS
175	174	5	9	8.1	5742	PASS
176	174	95	101	97.7	68978	PASS
177	176	5	9	6.3	4330	PASS

m/z	Abundance
36.00	1135.0
37.00	4731.0
38.00	4731.0
39.00	1776.0
40.00	192.0
43.90	1084.0
45.00	838.0
47.10	1135.0
48.00	481.0
49.00	5008.0
50.00	19320.0
51.00	6124.0
52.10	274.0
54.90	343.0
56.00	1747.0
57.00	2820.0
58.00	195.0
60.10	970.0
61.10	5409.0
62.10	4998.0
63.10	4299.0
63.90	504.0
64.90	683.0
66.00	123.0
66.80	207.0
68.00	9445.0
69.00	10012.0
70.00	727.0
72.00	658.0
73.00	4774.0
74.00	17344.0
75.10	50576.0
76.00	4193.0
76.90	485.0
77.70	259.0
78.90	4521.0
79.90	1160.0
80.90	4274.0
81.90	1145.0
82.90	138.0
87.00	3586.0
88.00	3160.0
90.90	490.0
92.00	3200.0
93.10	4489.0
94.10	11783.0
95.10	85632.0
96.10	5792.0
96.90	154.0
103.90	554.0
104.90	176.0
105.90	504.0
106.80	103.0
107.10	103.0
109.80	115.0
110.80	153.0
112.00	118.0
112.80	114.0
115.90	423.0
117.00	932.0
118.00	391.0
119.00	826.0
127.90	455.0
129.00	199.0
130.00	303.0
130.90	105.0
134.90	304.0
137.00	182.0
141.00	1228.0
142.10	221.0
143.00	1389.0
144.90	351.0
145.90	169.0
147.90	200.0
155.10	237.0
157.00	135.0
160.80	125.0
171.30	178.0
172.00	930.0
174.10	67400.0
175.10	5604.0
176.10	65672.0
177.00	4410.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.10	1159.0
37.00	4915.0
38.00	4838.0
39.00	1873.0
40.00	157.0
44.00	1221.0
45.00	889.0
47.10	1239.0
48.00	558.0
49.00	5120.0
50.00	20176.0
51.00	6253.0
52.00	282.0
54.90	310.0
56.00	1802.0
57.00	2938.0
58.00	147.0
60.10	1106.0
61.10	5496.0
62.00	5336.0
63.10	4473.0
63.90	487.0
64.90	631.0
65.90	123.0
66.80	183.0
68.00	9743.0
69.10	10434.0
70.00	889.0
72.00	640.0
73.00	4871.0
74.00	18280.0
75.10	53048.0
76.10	4269.0
76.90	510.0
78.90	4592.0
79.90	1249.0
80.90	4688.0
81.90	1253.0
82.90	119.0
86.00	125.0
87.00	3703.0
88.00	3242.0
90.90	552.0
92.00	3450.0
93.00	4829.0
94.10	12431.0
95.10	90120.0
96.10	5757.0
96.90	110.0
103.90	617.0
104.90	206.0
106.00	552.0
106.80	139.0
110.90	147.0
111.90	129.0
112.80	122.0
115.90	457.0
117.00	904.0
117.90	486.0
119.00	881.0
127.90	451.0
128.90	208.0
129.90	372.0
131.00	143.0
135.00	338.0
137.10	206.0
141.00	1415.0
142.10	199.0
143.00	1367.0
144.00	123.0
144.90	361.0
145.90	196.0
147.90	205.0
155.10	214.0
157.00	132.0
158.90	106.0
160.90	123.0
172.10	907.0
174.10	72992.0
175.10	5953.0
176.10	71432.0
177.00	4490.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.10	1108.0
37.00	4692.0
38.00	4459.0
39.00	1778.0
40.00	152.0
44.00	1183.0
45.00	876.0
47.10	1175.0
48.00	594.0
49.00	4519.0
50.00	19160.0
51.10	5822.0
51.90	274.0
53.00	103.0
55.00	307.0
56.00	1667.0
57.00	2797.0
58.10	101.0
60.00	1110.0
61.10	5219.0
62.00	5269.0
63.10	4173.0
63.90	443.0
65.10	549.0
65.90	117.0
68.00	9341.0
69.10	9896.0
70.00	909.0
72.00	560.0
73.10	4382.0
74.00	17648.0
75.10	50928.0
76.10	4165.0
77.00	546.0
78.90	4384.0
79.90	1236.0
80.90	4551.0
81.90	1232.0
86.10	138.0
87.00	3437.0
88.00	2956.0
90.90	520.0
92.00	3121.0
93.00	4581.0
94.10	11713.0
95.10	86464.0
96.10	5363.0
103.90	629.0
104.90	195.0
106.00	537.0
106.90	115.0
111.00	155.0
111.90	129.0
112.70	144.0
115.90	418.0
117.00	781.0
118.00	508.0
118.90	801.0
127.90	383.0
128.90	178.0
129.90	410.0
131.00	145.0
135.00	316.0
137.00	192.0
141.00	1471.0
142.00	139.0
143.00	1306.0
144.10	114.0
144.90	332.0
145.90	183.0
148.00	188.0
155.10	164.0
157.00	129.0
159.00	123.0
160.90	139.0
170.90	139.0
172.00	832.0
174.00	71520.0
175.10	5671.0
176.10	69832.0
177.00	4091.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

Scan 2882 (10.607 min): VU037259.D
BFB04

m/z	Abundance
36.00	194.0
37.80	102.0
43.90	295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04