

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031422\
 Data File : VU047550.D
 Acq On : 14 Mar 2022 21:16
 Operator : SY/MD
 Sample : N1906-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETNM5

Quant Time: Mar 15 06:16:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Mar 15 05:45:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	134395	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	131515	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	66899	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	39629	4.509	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.200%
7) Chloroethane-d5	1.919	69	39243	4.920	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.400%
11) 1,1-Dichloroethene-d2	2.571	65	17334	4.205	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.200%
20) 2-Butanone-d5	4.642	46	162289	64.172	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.340%
24) Chloroform-d	5.067	84	91392	4.735	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	5.706	65	52034	4.976	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.600%
32) Benzene-d6	5.732	84	175052	4.572	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
36) 1,2-Dichloropropane-d6	6.693	67	59633	4.953	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.000%
41) Toluene-d8	7.899	98	150933	4.205	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.000%
43) trans-1,3-Dichloroprop...	8.182	79	23357	4.615	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.200%
46) 2-Hexanone-d5	8.636	63	136148	51.890	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.780%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	58506	4.866	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.400%
66) 1,2-Dichlorobenzene-d4	12.195	152	67363	4.819	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.400%
Target Compounds					Qvalue	
42) Toluene	7.970	91	52650	1.634	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031422\
Data File : VU047550.D
Acq On : 14 Mar 2022 21:16
Operator : SY/MD
Sample : N1906-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETNM5

Quant Time: Mar 15 06:16:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Mar 15 05:45:04 2022
Response via : Initial Calibration

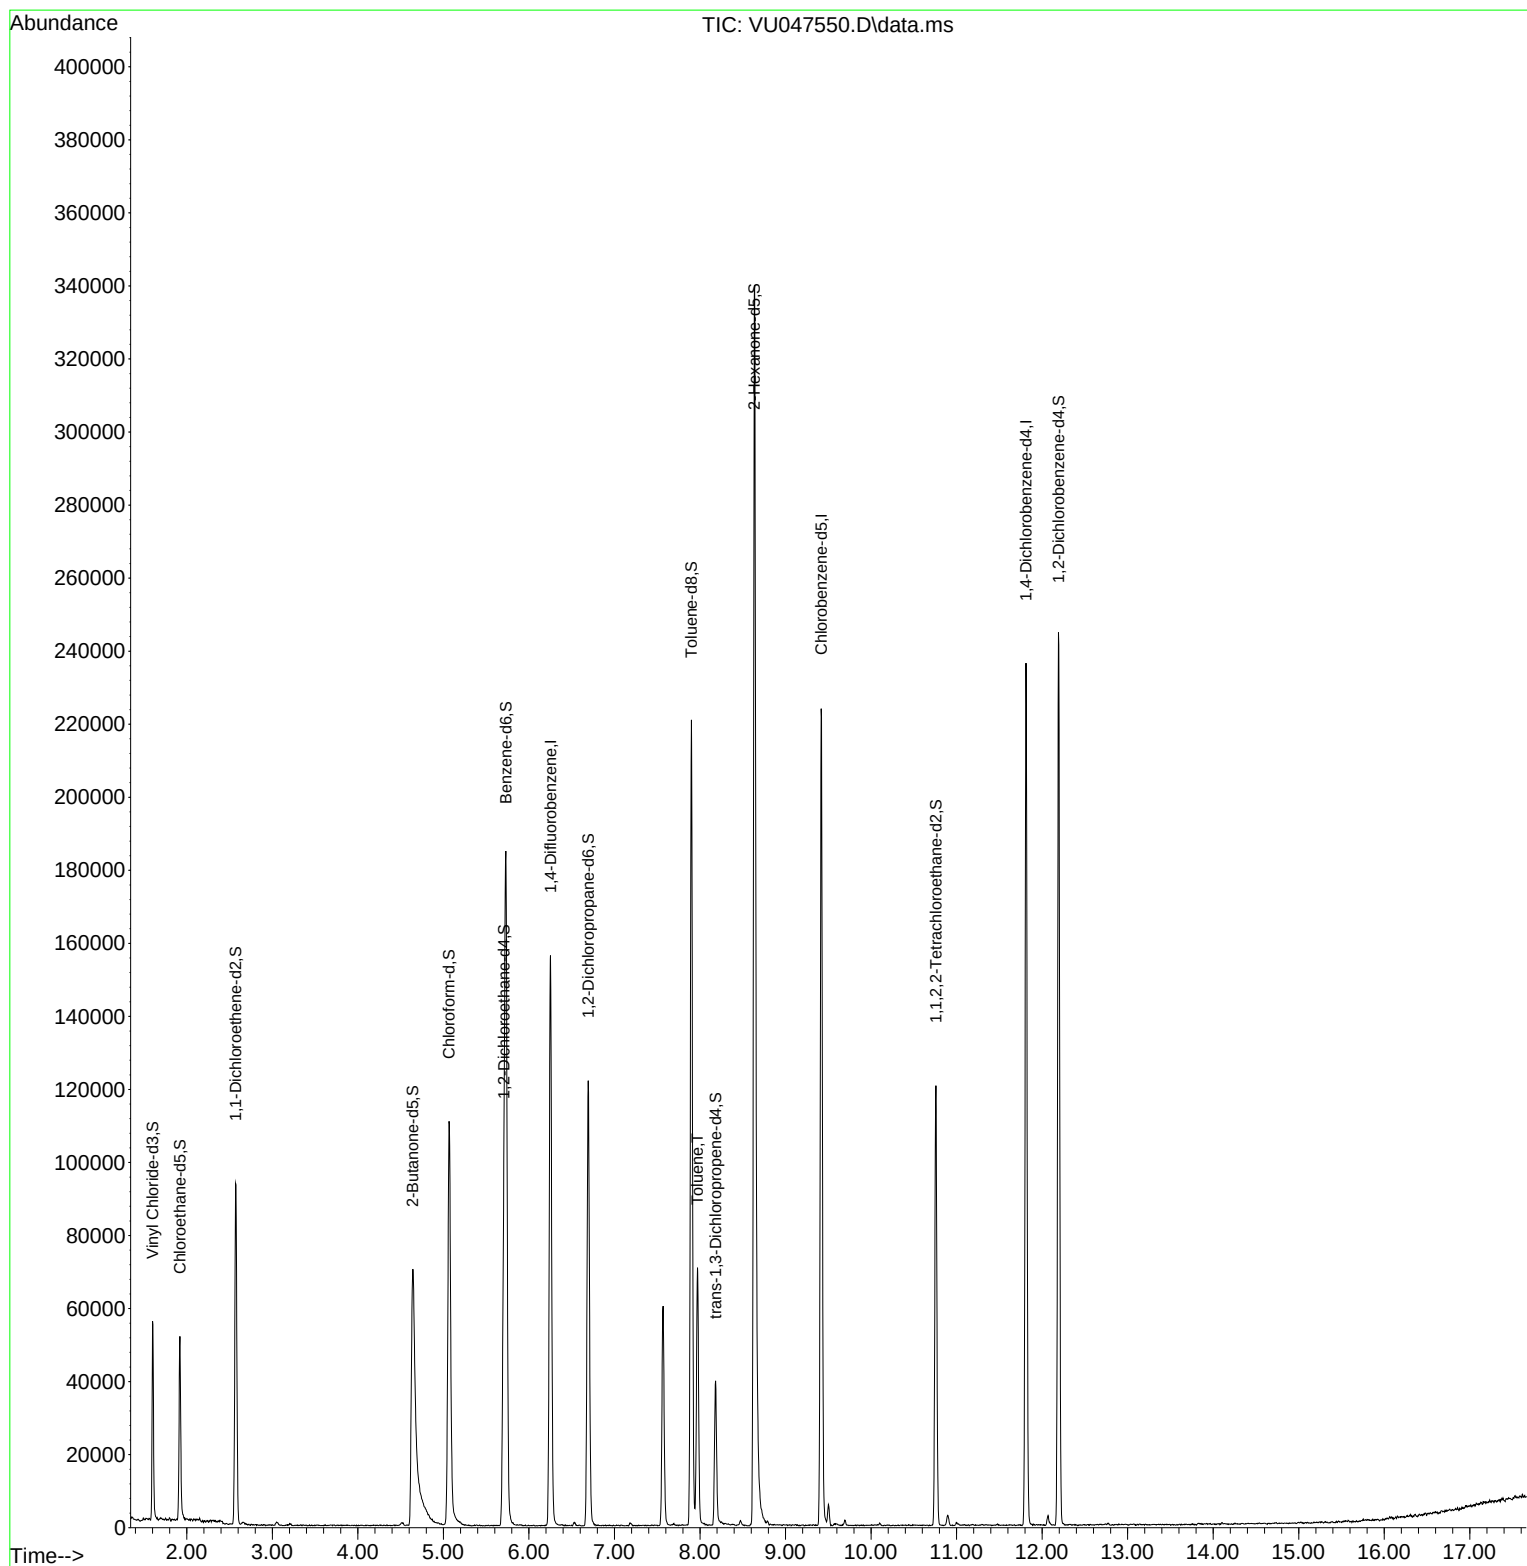

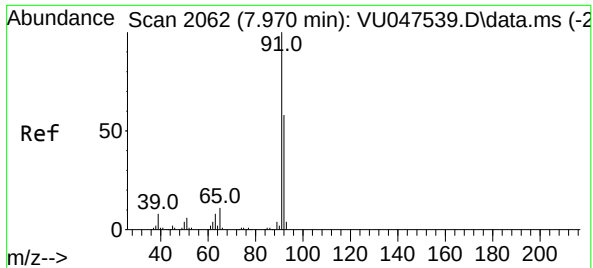

#42
Toluene
Concen: 1.634 ug/L
RT: 7.970 min Scan# 2062
Delta R.T. -0.000 min
Lab File: VU047550.D
Acq: 14 Mar 2022 21:16

Instrument :
MSVOA_U
ClientSampleId :
ETNM5

Tgt Ion: 91 Resp: 52650
Ion Ratio Lower Upper
91 100
92 58.0 40.2 74.6

