


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031422\
 Data File : VU047529.D
 Acq On : 14 Mar 2022 08:57
 Operator : SY/MD
 Sample : BFB067
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB067

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR031422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 18 01:27:05 2022

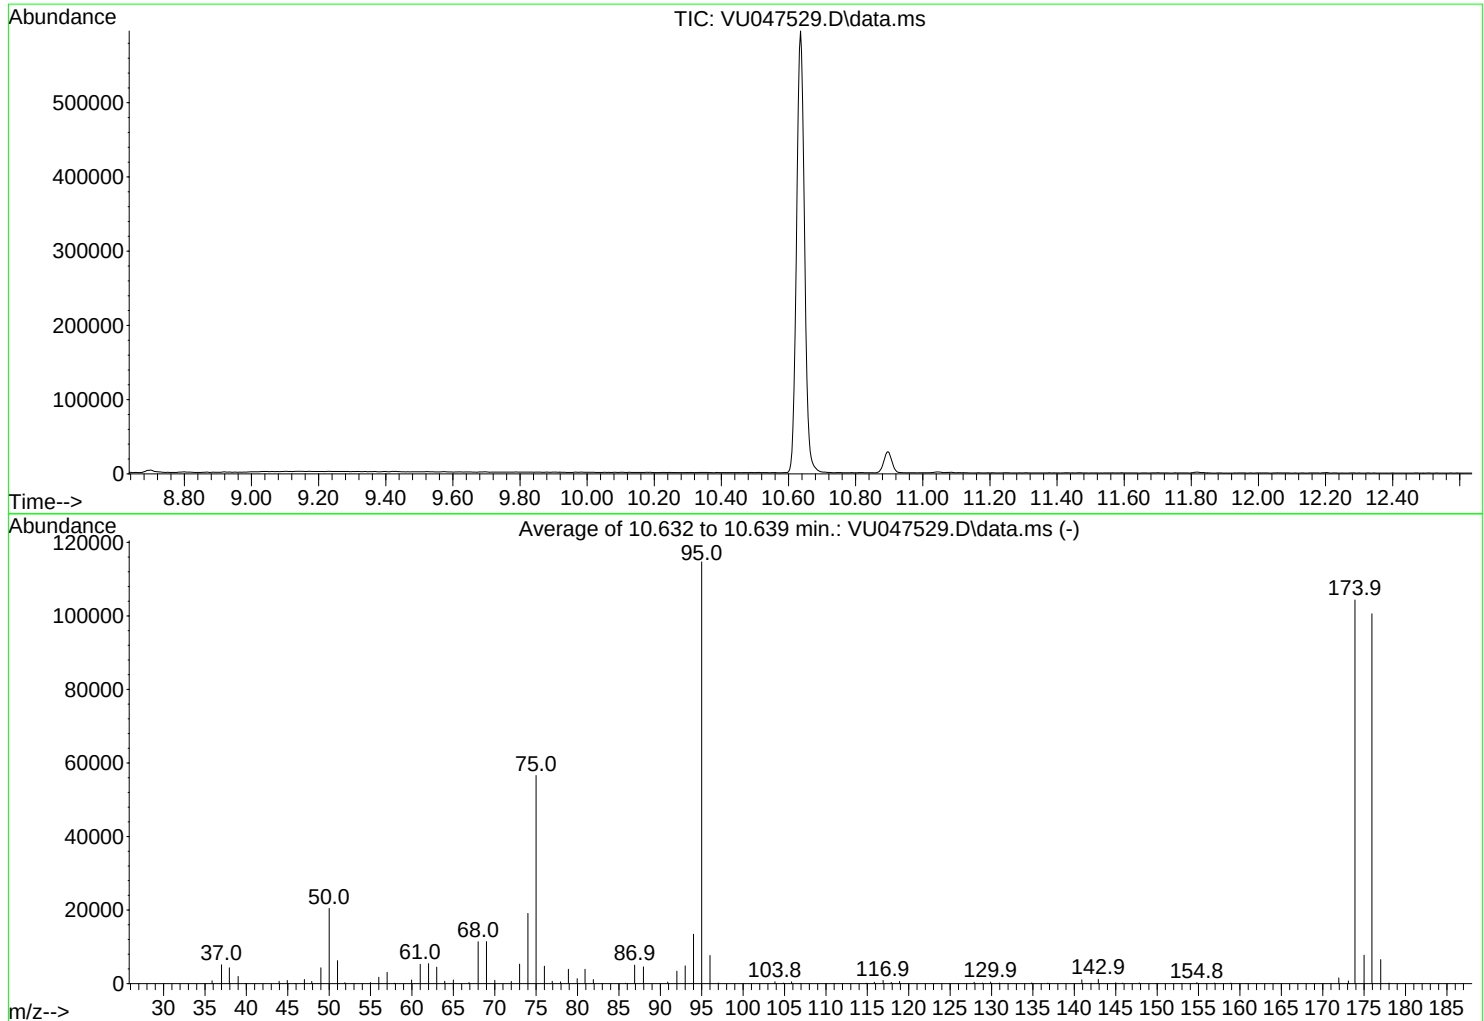

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	20451	PASS
75	95	30	80	49.3	56592	PASS
95	95	100	100	100.0	114696	PASS
96	95	5	9	6.7	7668	PASS
173	174	0.00	2	0.7	754	PASS
174	95	50	120	90.9	104315	PASS
175	174	5	9	7.4	7748	PASS
176	174	95	101	96.4	100597	PASS
177	176	5	9	6.5	6525	PASS

m/z	Abundance
35.90	901.0
37.90	331.0
39.90	275.0
43.90	208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	1708.0
37.00	5214.0
38.00	4770.0
39.00	1977.0
39.90	296.0
44.00	868.0
44.90	886.0
47.00	1068.0
47.90	592.0
49.00	4277.0
50.00	20664.0
51.00	6351.0
51.90	283.0
52.90	113.0
55.00	280.0
56.00	1803.0
57.00	3100.0
57.90	157.0
59.90	963.0
61.00	5305.0
62.00	5458.0
63.00	4615.0
63.90	640.0
65.00	1067.0
65.90	101.0
66.90	315.0
68.00	11416.0
69.00	11604.0
70.00	906.0
72.00	630.0
73.00	5211.0
74.00	18896.0
75.00	57008.0
76.00	4780.0
77.00	671.0
77.90	469.0
78.90	3948.0
80.00	1332.0
80.90	3852.0
81.90	1093.0
85.80	196.0
86.90	5055.0
87.90	4414.0
90.90	443.0
92.00	3323.0
93.00	4839.0
94.00	13513.0
95.00	113408.0
96.00	7617.0
97.00	191.0
103.80	523.0
104.90	170.0
105.90	528.0
106.90	137.0
114.80	123.0
115.80	376.0
116.90	861.0
117.90	359.0
118.90	577.0
127.90	397.0
128.90	226.0
129.90	436.0
130.90	193.0
134.80	207.0
136.80	171.0
140.90	998.0
142.00	144.0
142.90	1220.0
145.00	279.0
145.80	203.0
147.90	214.0
149.90	106.0
152.90	103.0
154.80	277.0
155.90	104.0
157.00	172.0
158.90	175.0
171.00	125.0
172.00	1741.0
173.90	101120.0
175.00	7639.0
175.90	97552.0
177.00	6600.0
178.00	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	1693.0
37.00	5318.0
38.00	4781.0
39.00	2026.0
39.90	296.0
44.00	887.0
44.90	902.0
47.00	1182.0
47.90	638.0
49.00	4437.0
50.00	21080.0
51.00	6427.0
51.90	284.0
52.90	112.0
55.00	296.0
56.00	1750.0
57.00	3134.0
57.90	154.0
60.00	1027.0
61.00	5405.0
62.00	5614.0
63.00	4643.0
64.00	677.0
65.00	1004.0
66.90	303.0
68.00	11838.0
69.00	11830.0
70.00	957.0
72.00	624.0
73.00	5553.0
74.00	19720.0
75.00	58144.0
76.00	4861.0
77.00	659.0
77.90	478.0
78.90	4068.0
79.90	1379.0
80.90	4048.0
81.90	1119.0
85.80	186.0
86.90	5257.0
87.90	4687.0
90.90	433.0
92.00	3487.0
93.00	4985.0
94.00	13739.0
95.00	118160.0
96.00	7870.0
97.00	169.0
103.80	534.0
104.90	182.0
105.80	532.0
106.90	116.0
114.80	152.0
115.90	384.0
116.90	891.0
117.90	365.0
118.90	628.0
127.90	435.0
128.90	192.0
129.90	436.0
130.90	209.0
134.80	213.0
136.80	191.0
140.90	1072.0
142.00	154.0
142.90	1207.0
145.00	267.0
145.80	175.0
147.90	236.0
149.90	108.0
152.90	110.0
154.80	306.0
157.00	183.0
158.90	192.0
171.00	113.0
171.90	1571.0
173.10	1126.0
173.90	107448.0
175.00	8015.0
176.00	103616.0
177.00	6732.0
178.00	197.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067

m/z	Abundance
35.90	1635.0
37.00	4921.0
38.00	4429.0
39.00	1935.0
39.90	313.0
44.00	860.0
45.00	869.0
45.90	100.0
47.00	1092.0
47.90	613.0
49.00	4233.0
50.00	19608.0
51.00	5973.0
51.90	254.0
52.90	101.0
55.00	288.0
56.00	1632.0
57.00	2982.0
57.90	145.0
60.00	1048.0
61.00	5096.0
62.00	5252.0
63.00	4245.0
64.00	626.0
65.00	957.0
66.90	295.0
68.00	10945.0
69.00	10894.0
70.00	908.0
72.00	522.0
73.00	5164.0
74.00	18744.0
75.00	54624.0
76.00	4599.0
76.90	638.0
78.00	433.0
78.90	3787.0
79.90	1318.0
80.90	3865.0
81.90	1047.0
82.90	103.0
86.00	177.0
86.90	4778.0
88.00	4560.0
90.90	381.0
92.00	3334.0
93.00	4709.0
94.00	13055.0
95.00	112520.0
96.00	7517.0
97.00	197.0
103.90	478.0
104.80	171.0
105.80	454.0
110.90	131.0
114.90	160.0
115.90	385.0
116.90	806.0
117.90	341.0
118.90	609.0
127.90	414.0
128.90	155.0
129.90	414.0
131.00	193.0
134.90	188.0
136.80	199.0
140.90	1017.0
142.00	149.0
142.90	1130.0
145.00	231.0
145.90	175.0
147.80	275.0
154.80	287.0
156.90	187.0
158.90	171.0
160.80	108.0
171.90	1444.0
173.10	1136.0
173.90	104376.0
175.00	7591.0
176.00	100624.0
177.00	6244.0
178.00	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB067