




Data File : VU030069.D
Acq On : 14 Mar 2019 13:16
Operator : JC/SP
Sample : K1838-13DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B2DL

Manual Integrations
APPROVED

MMDadoda
3/15/2019 9:22:25 AM

Quant Time: Mar 15 01:26:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 01:21:27 2019
Response via : Initial Calibration

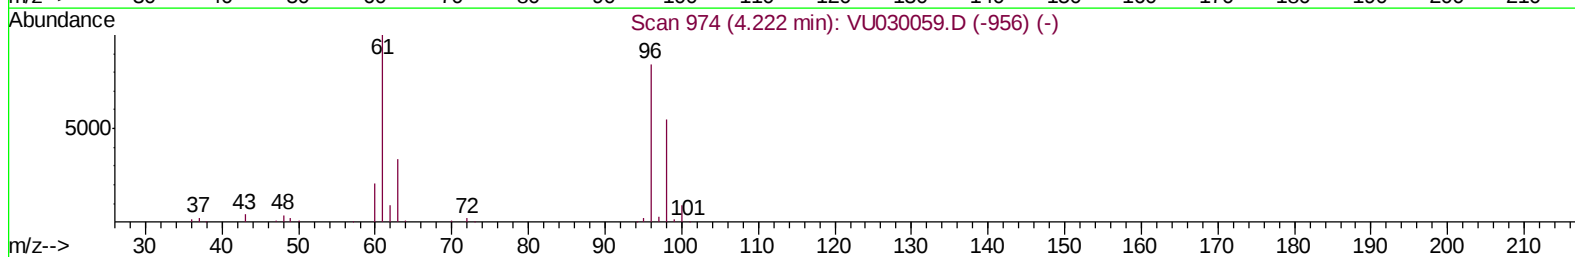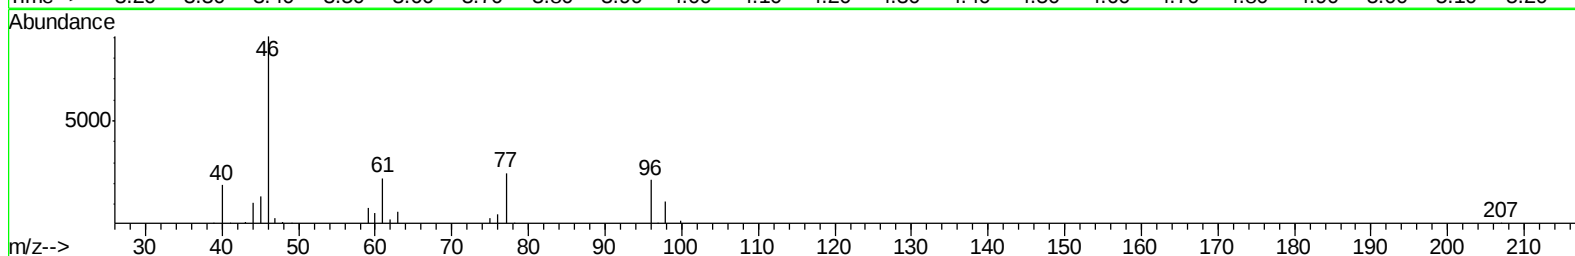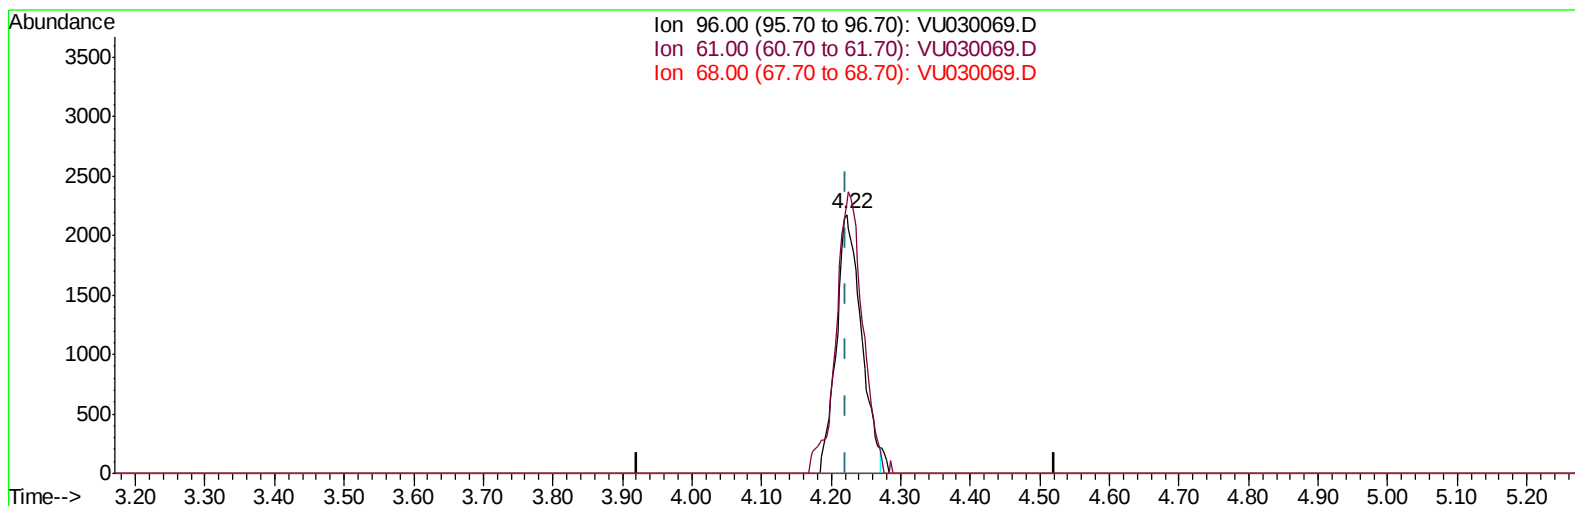

TIC: VU030069.D

(20) cis-1,2-Dichloroethene (T)

4.222min (+0.000) 1.48ug/L

response 5422

Ion	Exp%	Act%
96.00	100	100
61.00	115.50	104.59
68.00	0.00	0.00
0.00	0.00	0.00




Data File : VU030069.D
Acq On : 14 Mar 2019 13:16
Operator : JC/SP
Sample : K1838-13DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B2DL

Manual Integrations
APPROVED

MMDadoda
3/15/2019 9:22:25 AM

Quant Time: Mar 15 01:26:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 01:21:27 2019
Response via : Initial Calibration

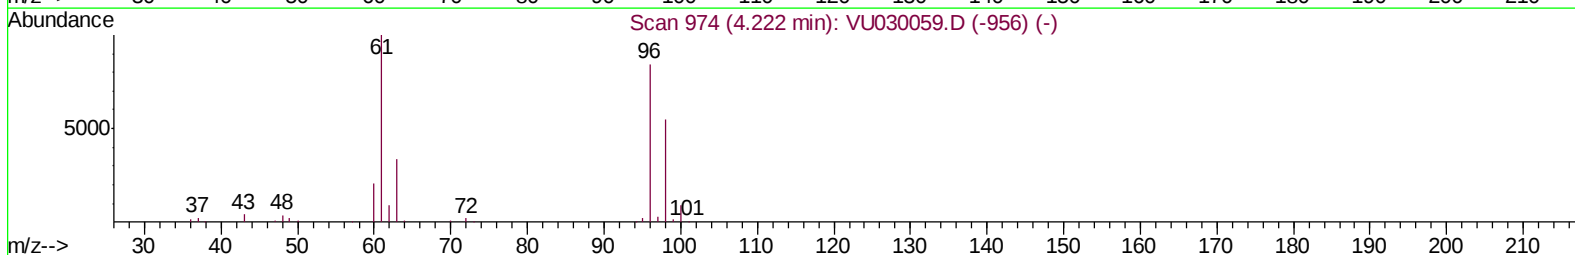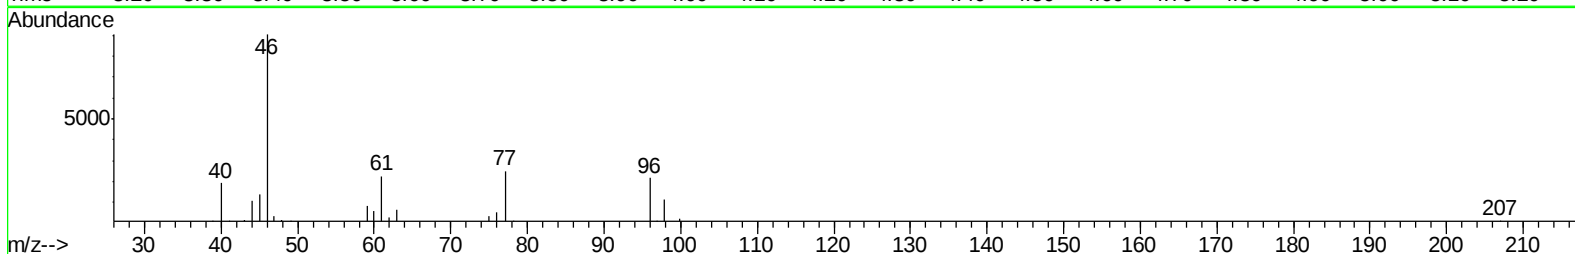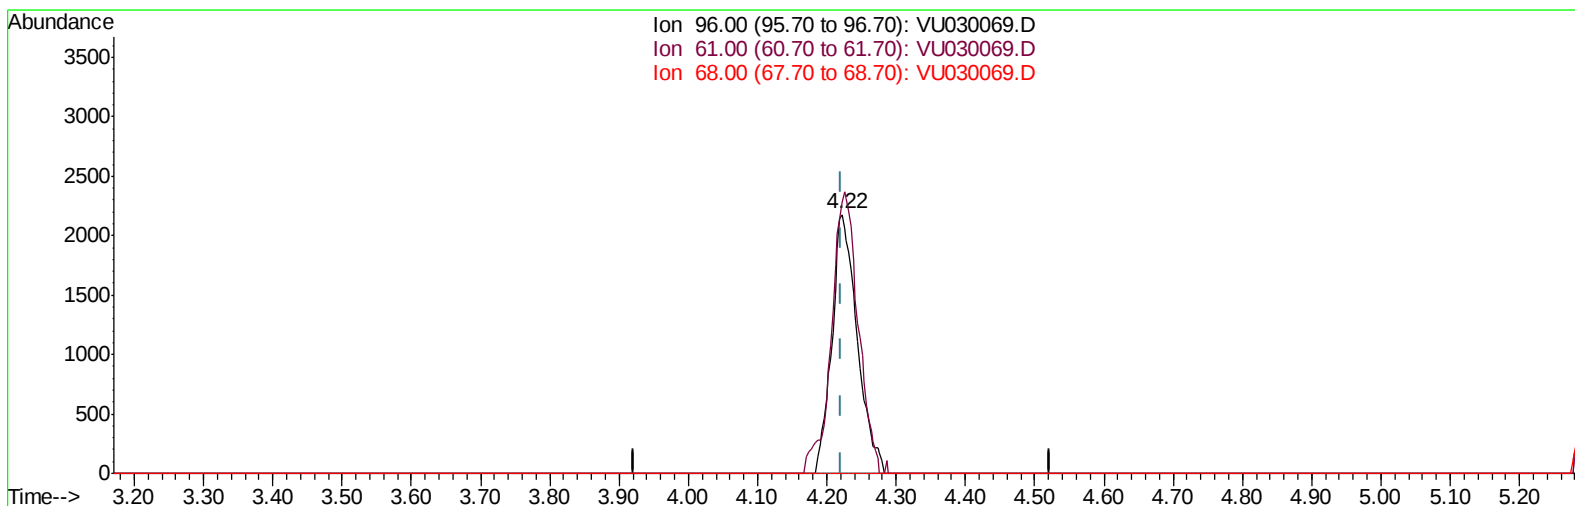

TIC: VU030069.D

(20) cis-1,2-Dichloroethene (T)

4.222min (+0.000) 1.51ug/L m

response 5518

Ion	Exp%	Act%
96.00	100	100
61.00	115.50	104.59
68.00	0.00	0.00
0.00	0.00	0.00

Data File : VU030069.D
Acq On : 14 Mar 2019 13:16
Operator : JC/SP
Sample : K1838-13DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B2DL

Manual Integrations
APPROVED

MMDadoda
3/15/2019 9:22:25 AM

Quant Time: Mar 15 02:17:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 01:21:27 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	470748	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	457850	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	219086	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	152044	48.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	97.66%
7) Chloroethane-d5	1.68	69	121323	48.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.54%
11) 1,1-Dichloroethene-d2	2.27	63	203487	36.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.42%
21) 2-Butanone-d5	4.17	46	209538	89.82	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.82%
24) Chloroform-d	4.65	84	256468	45.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.84%
26) 1,2-Dichloroethane-d4	5.31	65	154134	47.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.54%
32) Benzene-d6	5.34	84	564641	47.91	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.82%
36) 1,2-Dichloropropane-d6	6.33	67	173802	48.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.36%
41) Toluene-d8	7.56	98	514227	46.59	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.18%
43) trans-1,3-Dichloropropene-	7.85	79	77660	44.45	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.90%
47) 2-Hexanone-d5	8.31	63	179336	88.86	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	88.86%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	248320	44.80	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	206035	48.55	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.10%

Target Compounds					Qvalue
20) cis-1,2-Dichloroethene	4.22	96	5518m	1.509 ug/L	
46) Tetrachloroethene	8.22	164	95628	31.823 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU030069.D
Acq On : 14 Mar 2019 13:16
Operator : JC/SP
Sample : K1838-13DL 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B2DL

Manual Integrations
APPROVED

MMDadoda
3/15/2019 9:22:25 AM

Quant Time: Mar 15 02:17:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 15 01:21:27 2019
Response via : Initial Calibration

