

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030029.D
 Acq On : 13 Mar 2019 14:25
 Operator : JC/SP
 Sample : K1885-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1F0

Quant Time: Mar 14 03:07:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 14 01:36:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	553530	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	530817	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	259576	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	145277	39.68	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.36%
7) Chloroethane-d5	1.68	69	126855	42.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.84%
11) 1,1-Dichloroethene-d2	2.27	63	206814	31.29	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.58%
21) 2-Butanone-d5	4.17	46	246664	89.92	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.92%
24) Chloroform-d	4.65	84	283696	43.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.40%
26) 1,2-Dichloroethane-d4	5.31	65	171768	45.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.54%
32) Benzene-d6	5.34	84	609225	44.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.18%
36) 1,2-Dichloropropane-d6	6.33	67	191774	45.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.72%
41) Toluene-d8	7.56	98	552975	43.22	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.44%
43) trans-1,3-Dichloropropene-	7.85	79	86601	42.75	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.50%
47) 2-Hexanone-d5	8.31	63	214198	91.54	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.54%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	286084	44.52	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.04%
64) 1,2-Dichlorobenzene-d4	11.85	152	231495	46.04	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.08%


Target Compounds					Qvalue
3) Chloromethane	1.33	50	5415	1.403 ug/L	93
13) Acetone	2.32	43	8161	2.544 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030029.D
Acq On : 13 Mar 2019 14:25
Operator : JC/SP
Sample : K1885-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1F0

Quant Time: Mar 14 03:07:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 14 01:36:14 2019
Response via : Initial Calibration

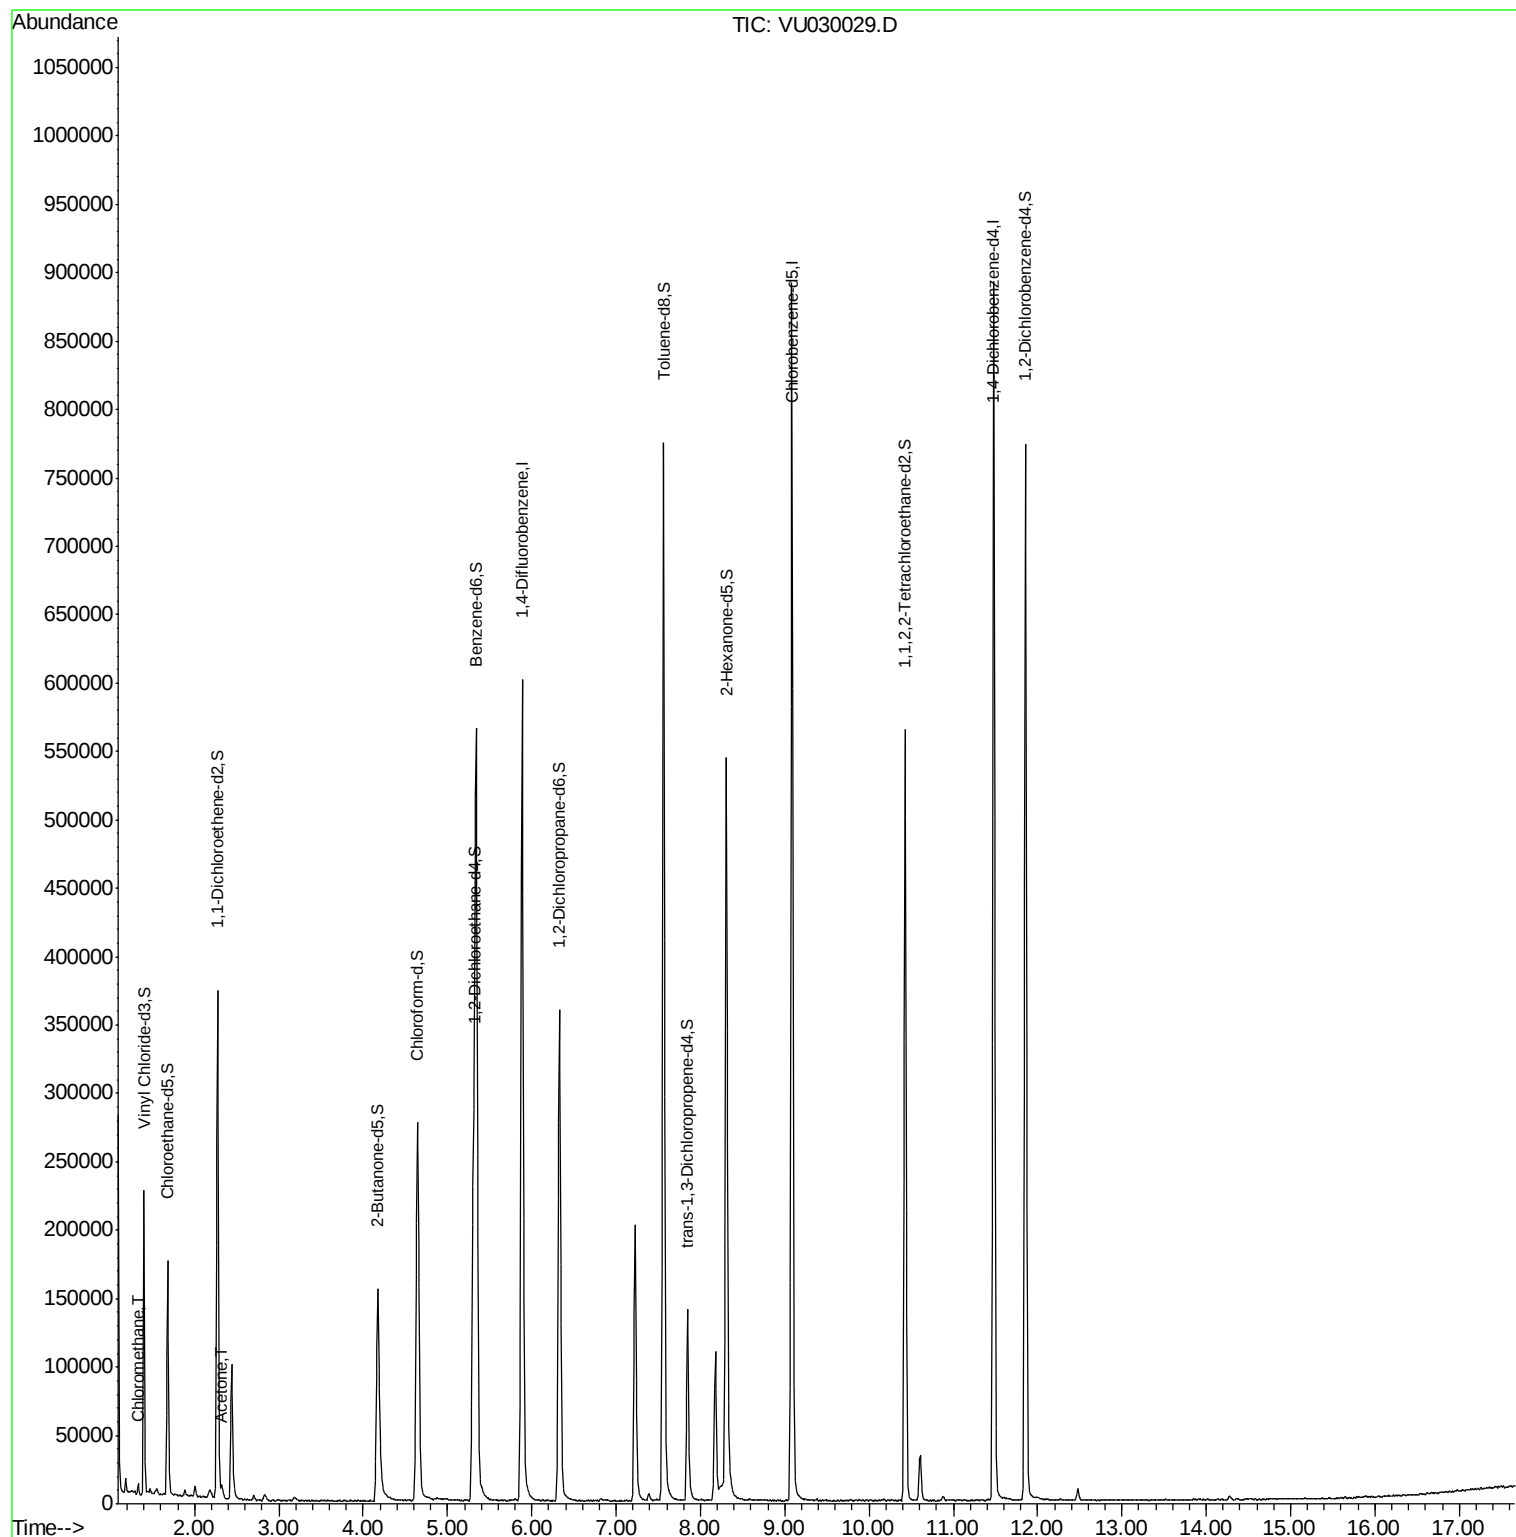

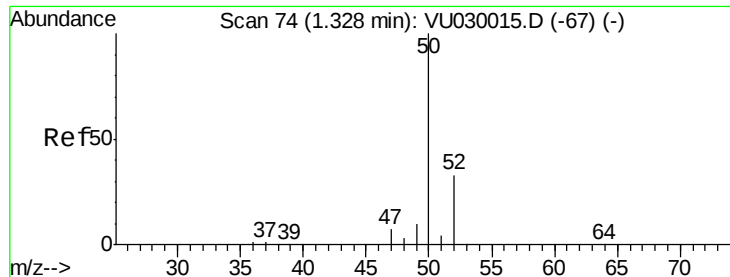

#3

Chloromethane

Concen: 1.403 ug/L

RT: 1.33 min Scan# 75

Delta R.T. 0.00 min

Lab File: VU030029.D

Acq: 13 Mar 2019 14:25

Instrument :

MSVOA_U

ClientSampleId :


BF1F0

Tgt Ion: 50 Resp: 5415

Ion Ratio Lower Upper




50 100

52 29.5 23.4 43.6

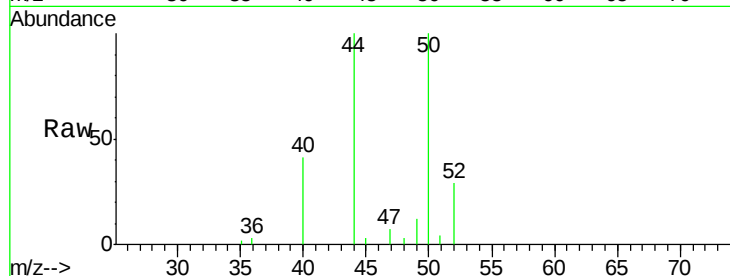

Abundance Ion 50.00 (49.70 to 50.70): VU0

Ion 52.00 (51.70 to 52.70): VU0

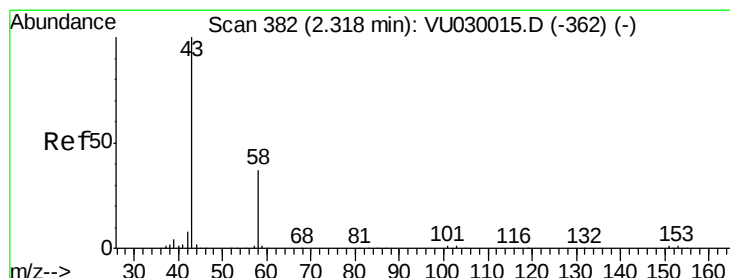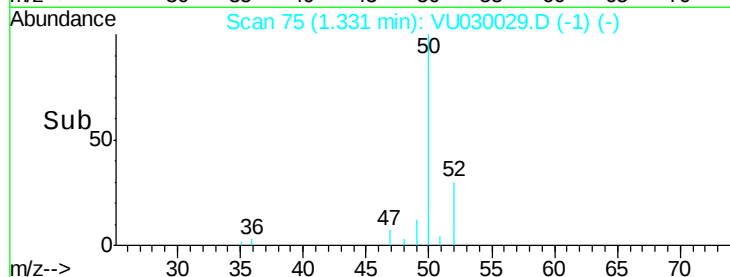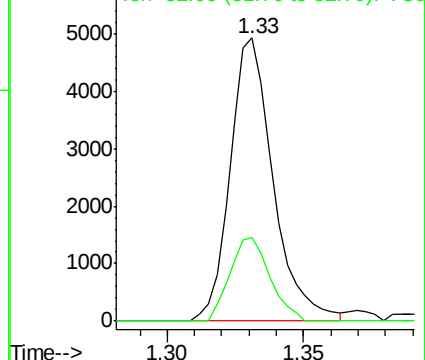

#13

Acetone

Concen: 2.544 ug/L

RT: 2.32 min Scan# 383

Delta R.T. 0.00 min

Lab File: VU030029.D


Acq: 13 Mar 2019 14:25

Tgt Ion: 43 Resp: 8161

Ion Ratio Lower Upper

43 100

58 36.6 0.0 73.0

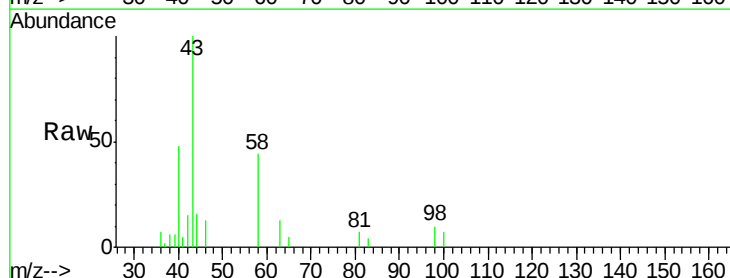

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

