

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030016.D
 Acq On : 13 Mar 2019 09:24
 Operator : JC/SP
 Sample : VU0315WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB	9574	8851	0.50%	0.063%
2	1.331	71	75	85	rVB	11436	12822	0.72%	0.091%
3	1.399	89	96	107	rBV	263690	267038	14.96%	1.893%
4	1.679	175	183	200	rVB	191244	244872	13.72%	1.736%
5	2.270	356	367	380	rBV	429190	651428	36.50%	4.617%
6	2.476	424	431	443	rVB2	1893	3257	0.18%	0.023%
7	2.563	455	458	461	rBV2	474	415	0.02%	0.003%
8	2.627	474	478	481	rBV4	477	445	0.02%	0.003%
9	2.701	493	501	503	rBV4	1275	1724	0.10%	0.012%
10	2.817	531	537	538	rBV2	1037	850	0.05%	0.006%
11	2.830	538	541	554	rVB4	2147	3331	0.19%	0.024%
12	2.984	582	589	596	rBV4	682	1312	0.07%	0.009%
13	3.103	623	626	629	rBV2	567	320	0.02%	0.002%
14	3.540	756	762	764	rVV	445	344	0.02%	0.002%
15	3.646	792	795	798	rBV	510	342	0.02%	0.002%
16	3.666	798	801	804	rBV2	528	354	0.02%	0.003%
17	3.813	838	847	850	rBV2	431	585	0.03%	0.004%
18	3.865	858	863	866	rBV	640	598	0.03%	0.004%
19	4.055	916	922	930	rVB2	535	819	0.05%	0.006%
20	4.170	946	958	986	rBV	158908	425776	23.85%	3.018%
21	4.505	1059	1062	1065	rBV3	612	392	0.02%	0.003%
22	4.547	1072	1075	1081	rVB4	629	515	0.03%	0.004%
23	4.643	1088	1105	1133	rBV	291353	700382	39.24%	4.964%
24	4.929	1192	1194	1195	rBV	611	312	0.02%	0.002%
25	5.045	1227	1230	1234	rVB2	512	309	0.02%	0.002%
26	5.241	1287	1291	1296	rBV4	452	405	0.02%	0.003%
27	5.338	1296	1321	1354	rBV2	610671	1784968	100.00%	12.651%
28	5.502	1371	1372	1376	rVB	609	320	0.02%	0.002%
29	5.601	1401	1403	1405	rBV	510	310	0.02%	0.002%
30	5.672	1420	1425	1428	rBV3	645	689	0.04%	0.005%
31	5.749	1444	1449	1451	rBV3	499	550	0.03%	0.004%
32	5.881	1477	1490	1526	rBV	535587	1087464	60.92%	7.707%
33	6.167	1574	1579	1581	rBV2	1464	1311	0.07%	0.009%
34	6.328	1614	1629	1651	rBV	380155	774279	43.38%	5.488%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030016.D
 Acq On : 13 Mar 2019 09:24
 Operator : JC/SP
 Sample : VU0315WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	6.588	1707	1710	1716	rBV	431	375	0.02%	0.003%
36	6.646	1721	1728	1729	rBV2	421	415	0.02%	0.003%
37	6.865	1790	1796	1797	rBV2	806	782	0.04%	0.006%
38	7.045	1844	1852	1855	rBV3	416	534	0.03%	0.004%
39	7.225	1896	1908	1938	rVV	222018	406648	22.78%	2.882%
40	7.347	1943	1946	1949	rVB2	489	360	0.02%	0.003%
41	7.437	1971	1974	1977	rBV2	555	422	0.02%	0.003%
42	7.463	1977	1982	1985	rBV4	1661	2028	0.11%	0.014%
43	7.563	1998	2013	2033	rBV	841605	1477381	82.77%	10.471%
44	7.845	2089	2101	2129	rBV	152859	274317	15.37%	1.944%
45	8.093	2176	2178	2182	rVB3	559	385	0.02%	0.003%
46	8.122	2182	2187	2188	rBV4	433	346	0.02%	0.002%
47	8.177	2190	2204	2215	rBV	42285	85294	4.78%	0.605%
48	8.305	2234	2244	2279	rVB	567944	994746	55.73%	7.050%
49	8.553	2319	2321	2325	rVB2	435	326	0.02%	0.002%
50	8.582	2327	2330	2335	rBV4	638	683	0.04%	0.005%
51	8.620	2335	2342	2351	rVV7	1101	2058	0.12%	0.015%
52	8.694	2361	2365	2369	rBV3	341	379	0.02%	0.003%
53	8.913	2427	2433	2437	rVB2	451	572	0.03%	0.004%
54	8.942	2437	2442	2446	rBV	507	479	0.03%	0.003%
55	9.087	2474	2487	2512	rBV	802657	1327586	74.38%	9.409%
56	9.254	2530	2539	2542	rBV6	1795	2148	0.12%	0.015%
57	9.286	2546	2549	2555	rVB	883	850	0.05%	0.006%
58	9.321	2555	2560	2565	rBV2	401	455	0.03%	0.003%
59	9.379	2572	2578	2586	rVB5	1664	2351	0.13%	0.017%
60	9.543	2624	2629	2633	rBV2	521	529	0.03%	0.004%
61	9.710	2674	2681	2685	rVB3	464	535	0.03%	0.004%
62	9.733	2685	2688	2691	rBV	448	307	0.02%	0.002%
63	9.775	2695	2701	2702	rBV3	1236	1034	0.06%	0.007%
64	9.797	2702	2708	2717	rVB7	1906	3183	0.18%	0.023%
65	9.948	2752	2755	2758	rBV4	524	357	0.02%	0.003%
66	10.170	2813	2824	2834	rBV5	2019	4213	0.24%	0.030%
67	10.321	2866	2871	2880	rVB5	767	1129	0.06%	0.008%
68	10.427	2892	2904	2928	rVV	580872	935191	52.39%	6.628%
69	10.607	2950	2960	2976	rBV	14520	27859	1.56%	0.197%
70	10.685	2980	2984	2988	rBV3	689	569	0.03%	0.004%
71	10.746	2999	3003	3009	rBV2	293	365	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030016.D
 Acq On : 13 Mar 2019 09:24
 Operator : JC/SP
 Sample : VU0315WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK57

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	10.881	3036	3045	3049	rBV4	1761	2433	0.14%	0.017%
73	11.115	3114	3118	3121	rVB3	506	406	0.02%	0.003%
74	11.170	3127	3135	3138	rBV2	505	705	0.04%	0.005%
75	11.215	3144	3149	3151	rBV2	349	354	0.02%	0.003%
76	11.321	3179	3182	3187	rVB2	677	512	0.03%	0.004%
77	11.421	3202	3213	3220	rBV7	4058	6099	0.34%	0.043%
78	11.482	3220	3232	3257	rBV	765739	1226921	68.74%	8.696%
79	11.778	3321	3324	3327	rVB3	535	410	0.02%	0.003%
80	11.858	3335	3349	3375	rBV	788670	1300484	72.86%	9.217%
81	12.112	3424	3428	3430	rBV2	535	412	0.02%	0.003%
82	12.199	3453	3455	3462	rVV4	447	409	0.02%	0.003%
83	12.295	3477	3485	3489	rVB4	801	954	0.05%	0.007%
84	12.318	3489	3492	3495	rBV	411	316	0.02%	0.002%
85	12.344	3495	3500	3502	rBV2	597	451	0.03%	0.003%
86	12.479	3536	3542	3552	rVB3	3726	5682	0.32%	0.040%
87	12.578	3569	3573	3583	rBV3	522	762	0.04%	0.005%
88	12.633	3583	3590	3592	rBV2	318	397	0.02%	0.003%
89	12.662	3596	3599	3605	rVB4	598	634	0.04%	0.004%
90	12.894	3664	3671	3682	rBV6	2748	5472	0.31%	0.039%
91	13.019	3707	3710	3717	rBV2	518	572	0.03%	0.004%
92	13.244	3775	3780	3783	rVB2	359	341	0.02%	0.002%
93	13.263	3783	3786	3793	rBV	503	611	0.03%	0.004%
94	13.443	3837	3842	3844	rBV2	710	477	0.03%	0.003%
95	13.517	3857	3865	3874	rBV7	3063	5877	0.33%	0.042%
96	13.762	3933	3941	3948	rBV8	2992	5684	0.32%	0.040%
97	13.951	3997	4000	4004	rBV3	487	419	0.02%	0.003%
98	14.000	4006	4015	4018	rBV5	3114	5477	0.31%	0.039%
99	14.446	4150	4154	4159	rBV2	497	547	0.03%	0.004%
100	15.684	4536	4539	4543	rBV3	998	736	0.04%	0.005%


Sum of corrected areas: 14109434

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030016.D
Acq On : 13 Mar 2019 09:24
Operator : JC/SP
Sample : VU0315WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK57

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

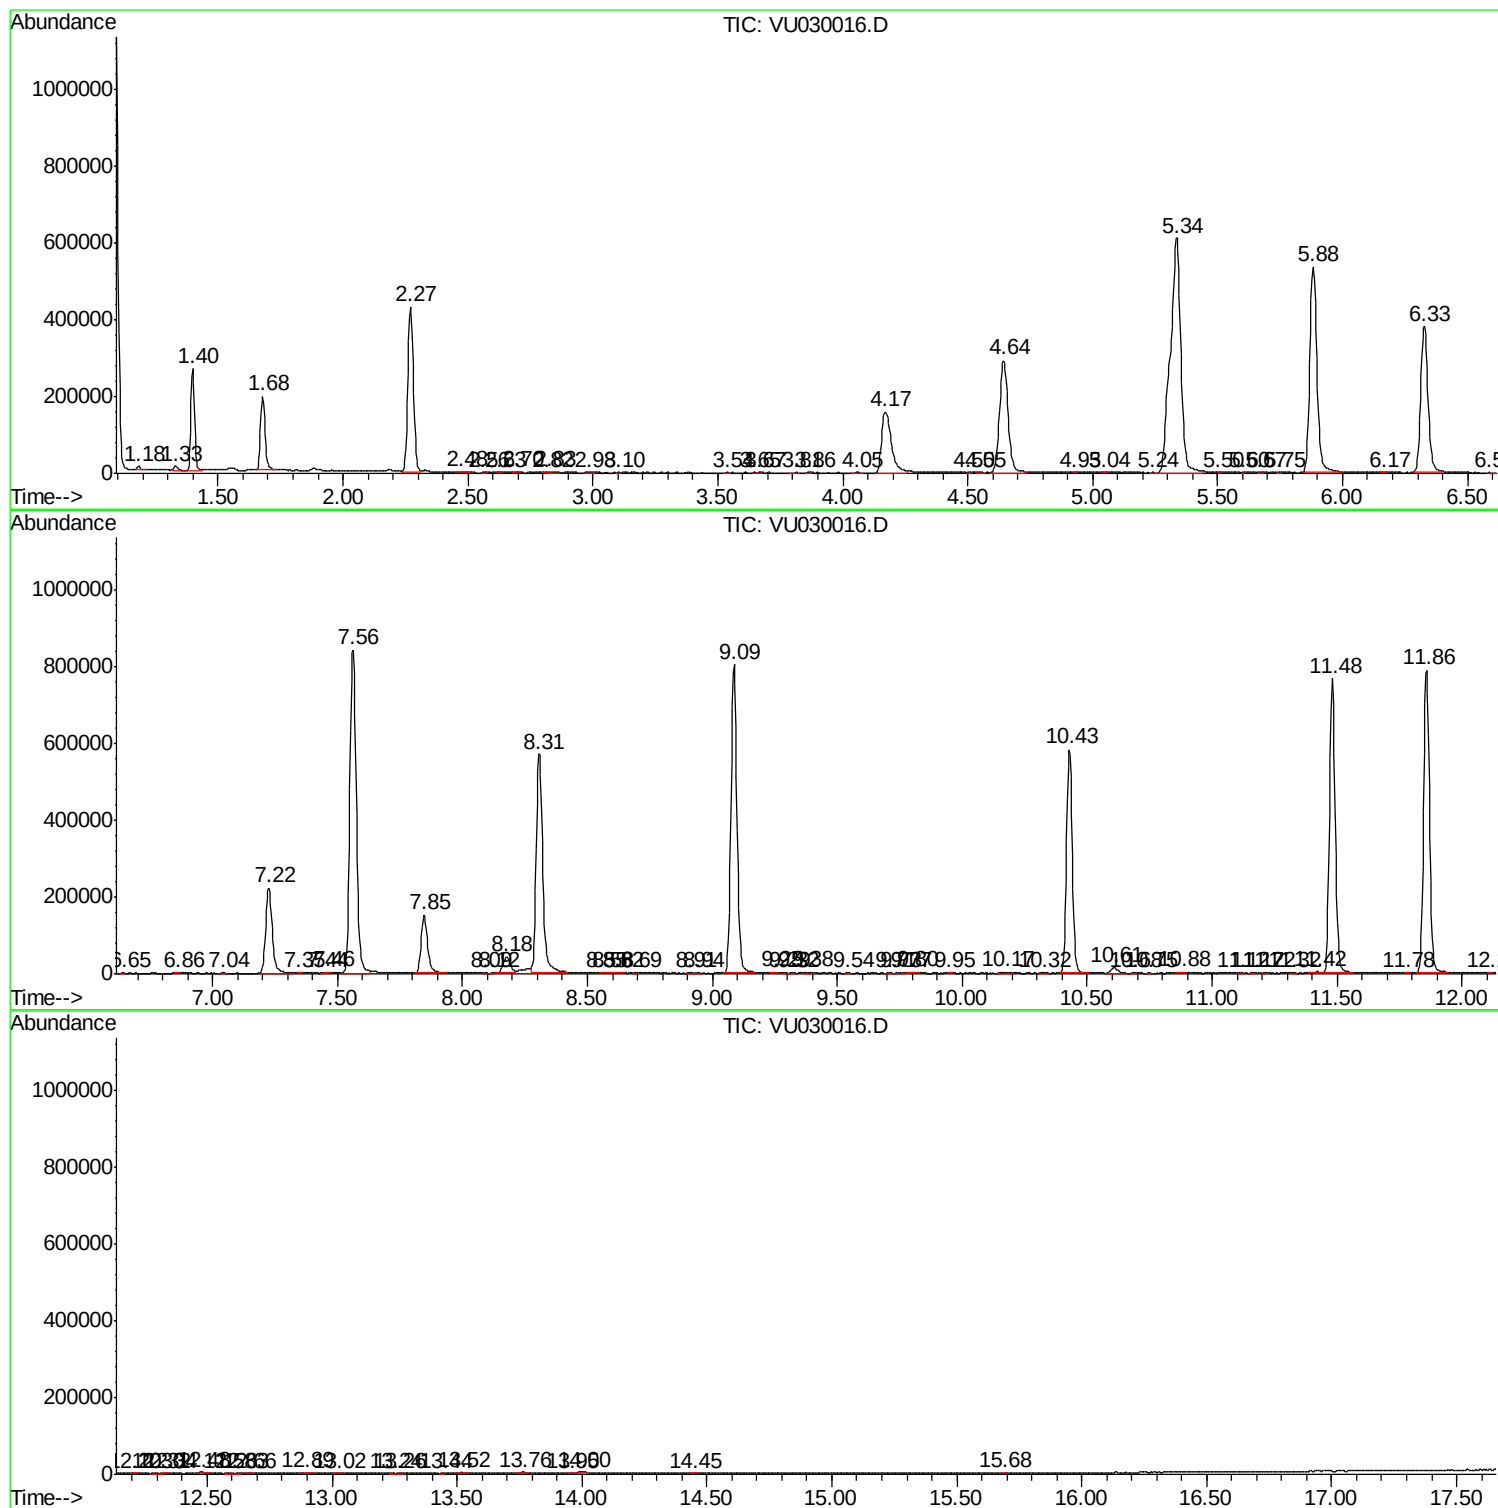

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030016.D
Acq On : 13 Mar 2019 09:24
Operator : JC/SP
Sample : VU0315WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK57

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030016.D
Acq On : 13 Mar 2019 09:24
Operator : JC/SP
Sample : VU0315WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK57

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
