

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030017.D
 Acq On : 13 Mar 2019 09:47
 Operator : JC/SP
 Sample : VU0315MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	39	rVB	10432	9649	0.55%	0.069%
2	1.399	89	96	110	rBV	257616	257271	14.68%	1.840%
3	1.679	175	183	203	rBV	183626	237574	13.56%	1.700%
4	2.273	356	368	381	rBV	407955	626107	35.73%	4.479%
5	2.540	446	451	453	rBV2	532	336	0.02%	0.002%
6	2.653	483	486	491	rVB3	559	546	0.03%	0.004%
7	2.701	491	501	508	rBV5	1530	2956	0.17%	0.021%
8	2.765	517	521	524	rBV3	467	351	0.02%	0.003%
9	2.814	532	536	538	rBV3	751	601	0.03%	0.004%
10	2.842	538	545	553	rVB3	2359	3363	0.19%	0.024%
11	2.990	585	591	596	rBV4	695	784	0.04%	0.006%
12	3.167	641	646	648	rBV	462	448	0.03%	0.003%
13	3.267	675	677	682	rVB2	511	339	0.02%	0.002%
14	3.293	682	685	688	rBV2	448	326	0.02%	0.002%
15	3.376	706	711	715	rVV2	338	372	0.02%	0.003%
16	3.399	715	718	725	rVB3	542	501	0.03%	0.004%
17	3.936	882	885	890	rVB3	421	355	0.02%	0.003%
18	4.174	946	959	990	rBV	165669	432911	24.71%	3.097%
19	4.585	1083	1087	1089	rBV2	446	379	0.02%	0.003%
20	4.646	1089	1106	1142	rBV	283800	681464	38.89%	4.875%
21	4.868	1172	1175	1177	rBV2	1090	690	0.04%	0.005%
22	4.984	1209	1211	1214	rBV2	559	401	0.02%	0.003%
23	5.096	1242	1246	1251	rVB3	503	380	0.02%	0.003%
24	5.132	1251	1257	1260	rVV4	558	666	0.04%	0.005%
25	5.167	1263	1268	1271	rVB3	407	379	0.02%	0.003%
26	5.235	1286	1289	1295	rVB3	463	374	0.02%	0.003%
27	5.338	1295	1321	1367	rBV2	598083	1752129	100.00%	12.534%
28	5.543	1383	1385	1390	rVB4	431	336	0.02%	0.002%
29	5.733	1442	1444	1447	rBV	519	332	0.02%	0.002%
30	5.804	1461	1466	1468	rBV4	357	366	0.02%	0.003%
31	5.884	1473	1491	1521	rBV	526206	1063769	60.71%	7.610%
32	6.061	1542	1546	1553	rVB2	709	680	0.04%	0.005%
33	6.183	1576	1584	1591	rVV7	1288	2601	0.15%	0.019%
34	6.260	1604	1608	1613	rBV3	385	319	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030017.D
 Acq On : 13 Mar 2019 09:47
 Operator : JC/SP
 Sample : VU0315MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	6.328	1614	1629	1658	rBV	376449	763486	43.57%	5.462%
36	6.579	1703	1707	1709	rBV	408	366	0.02%	0.003%
37	6.865	1790	1796	1797	rBV3	548	451	0.03%	0.003%
38	7.225	1896	1908	1934	rBV	219140	399279	22.79%	2.856%
39	7.376	1951	1955	1957	rBV3	465	333	0.02%	0.002%
40	7.389	1957	1959	1961	rVV3	648	364	0.02%	0.003%
41	7.402	1961	1963	1968	rVB	459	345	0.02%	0.002%
42	7.469	1979	1984	1991	rVB3	992	1148	0.07%	0.008%
43	7.563	1999	2013	2033	rBV	818641	1447359	82.61%	10.354%
44	7.845	2090	2101	2131	rBV	153106	270542	15.44%	1.935%
45	7.968	2135	2139	2142	rBV4	770	620	0.04%	0.004%
46	8.177	2188	2204	2217	rBV	91571	180903	10.32%	1.294%
47	8.308	2234	2245	2272	rVB	574601	987531	56.36%	7.064%
48	8.537	2312	2316	2321	rVB4	548	672	0.04%	0.005%
49	8.614	2336	2340	2353	rVB5	1789	2836	0.16%	0.020%
50	8.698	2363	2366	2368	rBV2	535	321	0.02%	0.002%
51	8.810	2396	2401	2404	rBV2	511	370	0.02%	0.003%
52	8.990	2454	2457	2459	rBV	459	366	0.02%	0.003%
53	9.087	2474	2487	2512	rBV	783000	1309696	74.75%	9.369%
54	9.328	2557	2562	2566	rBV3	611	726	0.04%	0.005%
55	9.382	2577	2579	2590	rVB5	1043	1499	0.09%	0.011%
56	9.479	2605	2609	2612	rVV	453	359	0.02%	0.003%
57	9.617	2649	2652	2659	rVV3	539	573	0.03%	0.004%
58	9.746	2686	2692	2694	rBV3	455	396	0.02%	0.003%
59	9.800	2706	2709	2717	rVB4	1181	1310	0.07%	0.009%
60	9.861	2723	2728	2731	rBV2	508	505	0.03%	0.004%
61	9.935	2746	2751	2754	rBV2	303	359	0.02%	0.003%
62	9.990	2763	2768	2771	rBV3	360	360	0.02%	0.003%
63	10.032	2776	2781	2783	rBV2	509	476	0.03%	0.003%
64	10.058	2787	2789	2793	rVV3	564	401	0.02%	0.003%
65	10.103	2797	2803	2808	rVB2	556	643	0.04%	0.005%
66	10.173	2818	2825	2835	rVB2	964	1682	0.10%	0.012%
67	10.344	2875	2878	2881	rBV3	518	447	0.03%	0.003%
68	10.427	2891	2904	2922	rBV	584729	932787	53.24%	6.673%
69	10.566	2942	2947	2949	rBV2	773	510	0.03%	0.004%
70	10.604	2949	2959	2974	rVV	18835	33939	1.94%	0.243%
71	10.816	3021	3025	3028	rBV3	449	382	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030017.D
 Acq On : 13 Mar 2019 09:47
 Operator : JC/SP
 Sample : VU0315MBL01
 Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK58

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	10.878	3033	3044	3051	rBV6	1985	3770	0.22%	0.027%
73	11.029	3087	3091	3096	rBV2	644	664	0.04%	0.005%
74	11.080	3104	3107	3112	rVB3	872	644	0.04%	0.005%
75	11.231	3151	3154	3159	rBV3	525	382	0.02%	0.003%
76	11.411	3205	3210	3211	rBV4	1565	1070	0.06%	0.008%
77	11.479	3219	3231	3250	rBV	764780	1235613	70.52%	8.839%
78	11.810	3331	3334	3336	rBV2	551	390	0.02%	0.003%
79	11.855	3336	3348	3379	rVV	790092	1294284	73.87%	9.259%
80	11.984	3385	3388	3390	rBV3	1067	560	0.03%	0.004%
81	12.080	3413	3418	3422	rVB3	542	537	0.03%	0.004%
82	12.424	3521	3525	3526	rBV	441	326	0.02%	0.002%
83	12.476	3532	3541	3558	rVB3	3483	6676	0.38%	0.048%
84	12.556	3559	3566	3569	rBV2	540	642	0.04%	0.005%
85	12.865	3655	3662	3664	rBV	583	566	0.03%	0.004%
86	12.900	3667	3673	3678	rVV5	1306	1713	0.10%	0.012%
87	13.102	3733	3736	3739	rBV2	542	374	0.02%	0.003%
88	13.138	3743	3747	3749	rBV2	692	561	0.03%	0.004%
89	13.318	3800	3803	3809	rVB3	415	371	0.02%	0.003%
90	13.459	3845	3847	3853	rBV2	360	362	0.02%	0.003%
91	13.614	3892	3895	3899	rVB2	597	447	0.03%	0.003%
92	13.710	3922	3925	3929	rBV2	452	319	0.02%	0.002%
93	13.755	3936	3939	3943	rBV2	628	536	0.03%	0.004%
94	13.781	3944	3947	3950	rVV2	704	499	0.03%	0.004%
95	13.845	3961	3967	3970	rBV3	539	689	0.04%	0.005%
96	13.974	4004	4007	4011	rBV3	376	377	0.02%	0.003%
97	14.003	4011	4016	4018	rBV3	794	721	0.04%	0.005%
98	14.167	4064	4067	4069	rBV	724	459	0.03%	0.003%
99	14.234	4084	4088	4093	rBV3	621	570	0.03%	0.004%
100	14.723	4237	4240	4243	rBV2	645	382	0.02%	0.003%


Sum of corrected areas: 13978901

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030017.D
Acq On : 13 Mar 2019 09:47
Operator : JC/SP
Sample : VU0315MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

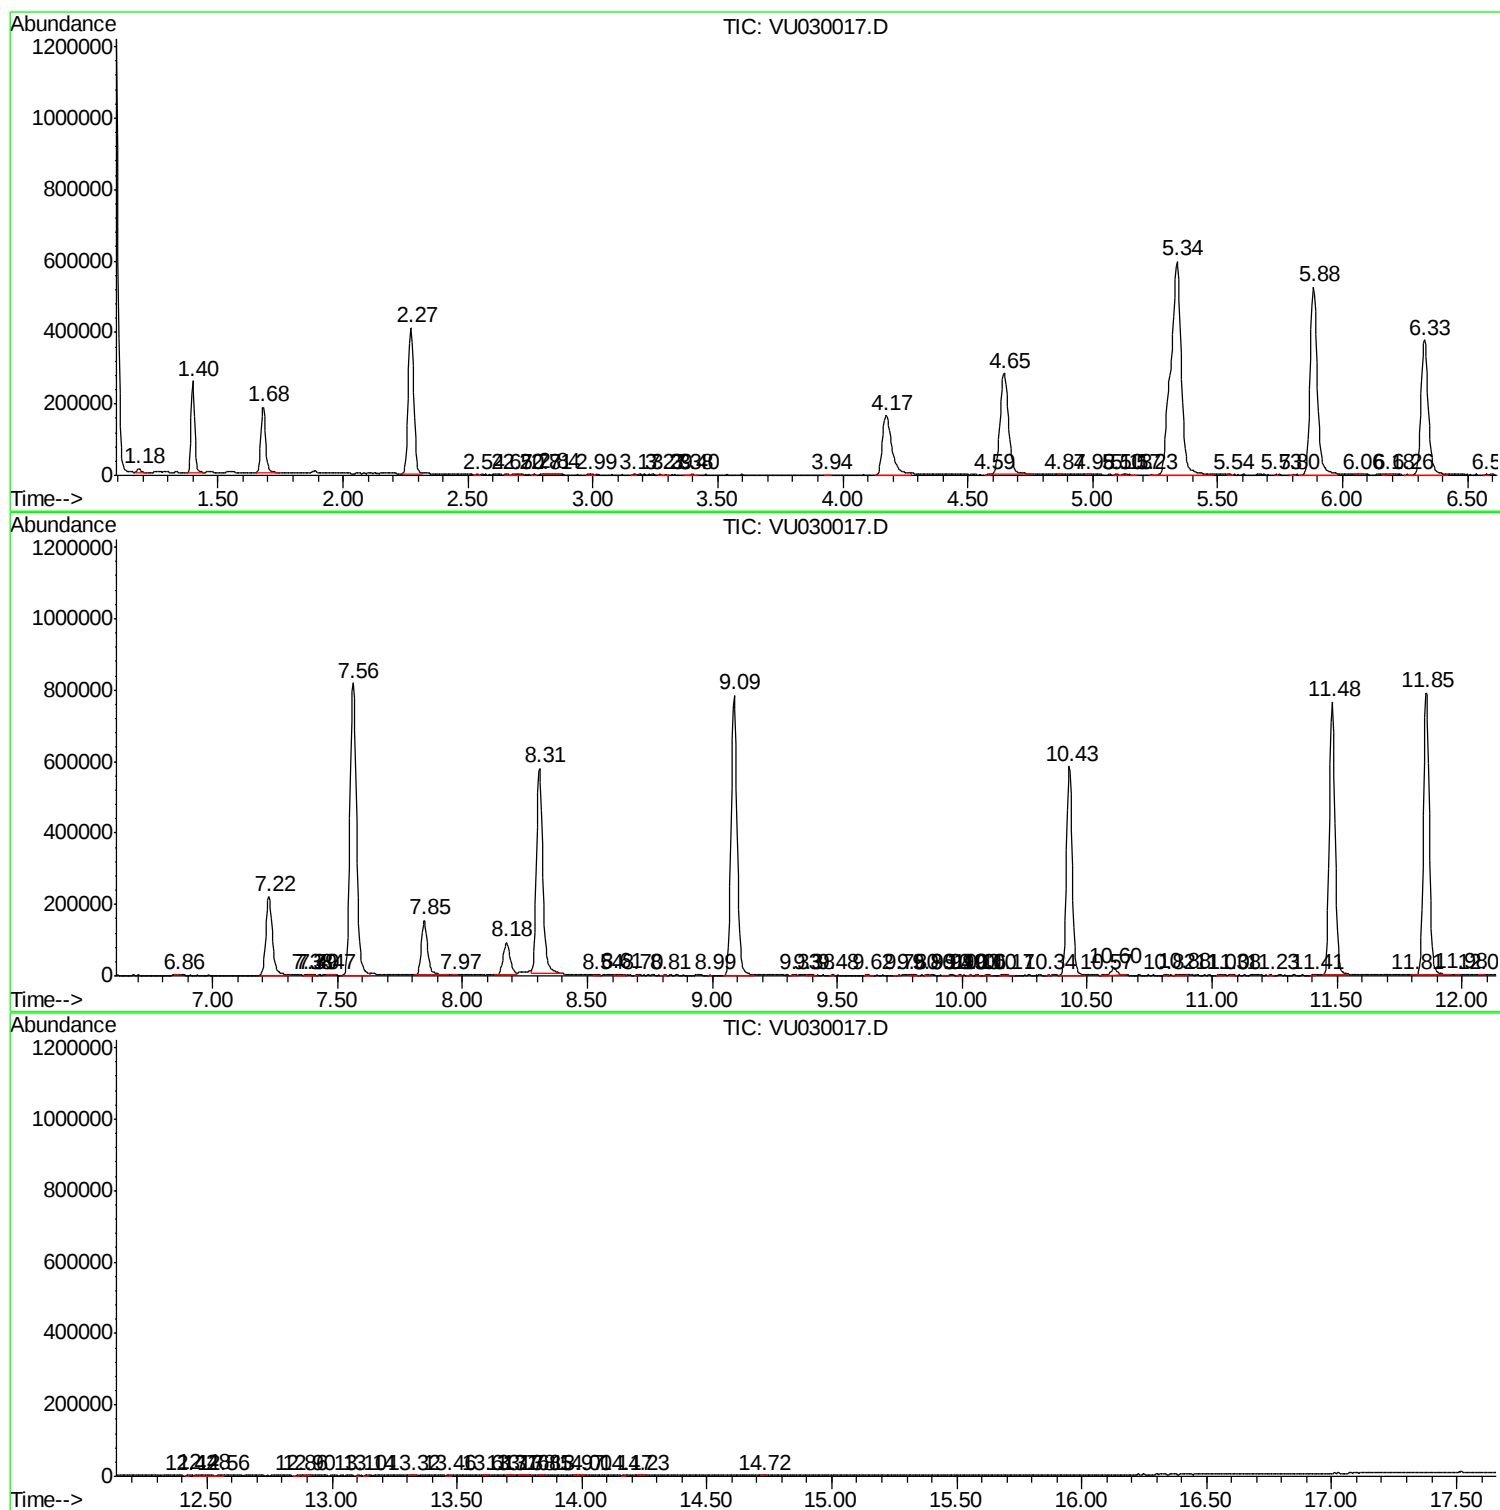

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030017.D
Acq On : 13 Mar 2019 09:47
Operator : JC/SP
Sample : VU0315MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030017.D
Acq On : 13 Mar 2019 09:47
Operator : JC/SP
Sample : VU0315MBL01
Misc : 5.00g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK58

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc