

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030020.D
 Acq On : 13 Mar 2019 10:55
 Operator : JC/SP
 Sample : K1734-15DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	34	rVB2	8796	7500	0.47%	0.055%
2	1.399	89	96	110	rBV	228735	231118	14.39%	1.704%
3	1.682	176	184	198	rVB	167627	213441	13.29%	1.574%
4	2.273	356	368	382	rBV	372895	572182	35.62%	4.219%
5	2.440	416	420	425	rBV5	1111	1080	0.07%	0.008%
6	2.694	496	499	500	rBV	811	376	0.02%	0.003%
7	2.762	513	520	522	rBV2	444	545	0.03%	0.004%
8	2.871	547	554	557	rBV	527	516	0.03%	0.004%
9	2.993	584	592	595	rVV4	706	972	0.06%	0.007%
10	3.010	595	597	602	rVB2	629	390	0.02%	0.003%
11	3.048	602	609	614	rVB3	620	705	0.04%	0.005%
12	3.331	692	697	698	rBV	775	535	0.03%	0.004%
13	3.386	709	714	717	rVV	525	499	0.03%	0.004%
14	3.466	735	739	742	rVB	482	382	0.02%	0.003%
15	3.685	804	807	810	rBV2	507	358	0.02%	0.003%
16	3.752	823	828	832	rBV2	385	385	0.02%	0.003%
17	3.887	866	870	879	rVB2	419	521	0.03%	0.004%
18	4.087	926	932	936	rBV	550	733	0.05%	0.005%
19	4.173	945	959	990	rBV	145675	386973	24.09%	2.853%
20	4.434	1037	1040	1046	rVB3	495	480	0.03%	0.004%
21	4.498	1056	1060	1064	rBV4	454	355	0.02%	0.003%
22	4.530	1068	1070	1073	rVB	569	346	0.02%	0.003%
23	4.646	1089	1106	1134	rBV	262414	625429	38.93%	4.612%
24	5.337	1298	1321	1364	rBV2	546411	1606431	100.00%	11.845%
25	5.608	1400	1405	1409	rBV	591	684	0.04%	0.005%
26	5.669	1417	1424	1427	rVB3	884	815	0.05%	0.006%
27	5.807	1464	1467	1471	rBV3	613	510	0.03%	0.004%
28	5.884	1476	1491	1532	rBV	503588	1028600	64.03%	7.584%
29	6.186	1577	1585	1597	rVB5	3368	6927	0.43%	0.051%
30	6.263	1605	1609	1610	rBV2	466	358	0.02%	0.003%
31	6.328	1615	1629	1660	rBV	342716	703382	43.79%	5.186%
32	6.505	1681	1684	1689	rVB2	630	593	0.04%	0.004%
33	6.646	1726	1728	1737	rVB	447	433	0.03%	0.003%
34	6.765	1760	1765	1769	rVB2	348	358	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030020.D
 Acq On : 13 Mar 2019 10:55
 Operator : JC/SP
 Sample : K1734-15DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	6.852	1787	1792	1793	rBV2	612	547	0.03%	0.004%
36	7.096	1864	1868	1872	rVB3	458	445	0.03%	0.003%
37	7.119	1872	1875	1877	rBV2	547	375	0.02%	0.003%
38	7.160	1883	1888	1892	rBV2	416	481	0.03%	0.004%
39	7.225	1892	1908	1936	rBV	199409	365908	22.78%	2.698%
40	7.443	1970	1976	1979	rBV3	373	413	0.03%	0.003%
41	7.472	1980	1985	1987	rVB3	832	669	0.04%	0.005%
42	7.562	2000	2013	2047	rBV	750582	1330735	82.84%	9.812%
43	7.845	2091	2101	2123	rBV	136159	240396	14.96%	1.773%
44	8.177	2190	2204	2210	rBV2	86930	159995	9.96%	1.180%
45	8.225	2211	2219	2234	rVV	346078	610959	38.03%	4.505%
46	8.308	2235	2245	2278	rVB	525827	922032	57.40%	6.799%
47	8.591	2330	2333	2336	rVB2	623	346	0.02%	0.003%
48	8.781	2389	2392	2398	rVB3	576	443	0.03%	0.003%
49	8.823	2401	2405	2406	rBV2	573	433	0.03%	0.003%
50	8.958	2444	2447	2451	rVB	540	330	0.02%	0.002%
51	8.993	2455	2458	2462	rBV2	565	445	0.03%	0.003%
52	9.086	2474	2487	2519	rBV	752590	1259552	78.41%	9.287%
53	9.305	2549	2555	2557	rBV2	510	556	0.03%	0.004%
54	9.386	2575	2580	2590	rVB5	851	1181	0.07%	0.009%
55	9.504	2613	2617	2622	rVB3	380	367	0.02%	0.003%
56	9.562	2632	2635	2637	rBV2	647	439	0.03%	0.003%
57	9.617	2649	2652	2658	rVB3	696	715	0.04%	0.005%
58	9.733	2685	2688	2693	rVB2	468	423	0.03%	0.003%
59	9.778	2697	2702	2705	rBV3	602	565	0.04%	0.004%
60	9.894	2736	2738	2743	rVB2	449	361	0.02%	0.003%
61	9.987	2764	2767	2770	rVB	592	371	0.02%	0.003%
62	10.032	2775	2781	2787	rBV2	590	865	0.05%	0.006%
63	10.131	2808	2812	2815	rBV3	485	344	0.02%	0.003%
64	10.170	2821	2824	2827	rBV2	541	396	0.02%	0.003%
65	10.215	2833	2838	2841	rBV2	472	451	0.03%	0.003%
66	10.427	2892	2904	2930	rBV	531128	853992	53.16%	6.297%
67	10.607	2950	2960	2974	rVB	20262	36750	2.29%	0.271%
68	10.684	2981	2984	2988	rVB2	583	377	0.02%	0.003%
69	10.791	3014	3017	3022	rBV2	447	462	0.03%	0.003%
70	10.871	3032	3042	3043	rBV3	2028	2064	0.13%	0.015%
71	10.977	3072	3075	3078	rBV2	683	538	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030020.D
 Acq On : 13 Mar 2019 10:55
 Operator : JC/SP
 Sample : K1734-15DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	11.006	3082	3084	3089	rBV3	297	350	0.02%	0.003%
73	11.083	3103	3108	3113	rVB3	796	882	0.05%	0.007%
74	11.128	3117	3122	3126	rVB2	631	599	0.04%	0.004%
75	11.209	3143	3147	3151	rBV3	488	507	0.03%	0.004%
76	11.247	3156	3159	3162	rBV2	533	413	0.03%	0.003%
77	11.411	3201	3210	3211	rBV3	1175	1093	0.07%	0.008%
78	11.479	3219	3231	3250	rBV	736247	1170088	72.84%	8.628%
79	11.858	3336	3349	3371	rBV	707392	1177169	73.28%	8.680%
80	12.189	3449	3452	3454	rBV2	540	351	0.02%	0.003%
81	12.295	3481	3485	3488	rBV2	593	454	0.03%	0.003%
82	12.337	3495	3498	3500	rBV2	586	364	0.02%	0.003%
83	12.408	3516	3520	3526	rBV3	402	451	0.03%	0.003%
84	12.475	3531	3541	3553	rVB2	4139	8006	0.50%	0.059%
85	12.598	3570	3579	3581	rBV3	684	906	0.06%	0.007%
86	12.755	3622	3628	3632	rBV3	547	743	0.05%	0.005%
87	13.337	3806	3809	3813	rVB2	508	408	0.03%	0.003%
88	13.479	3850	3853	3857	rVB	619	471	0.03%	0.003%
89	13.765	3937	3942	3947	rBV3	971	1236	0.08%	0.009%
90	13.864	3971	3973	3979	rVB3	510	430	0.03%	0.003%
91	13.897	3980	3983	3986	rBV2	537	364	0.02%	0.003%
92	14.485	4162	4166	4168	rBV	540	452	0.03%	0.003%
93	14.543	4178	4184	4187	rBV3	619	751	0.05%	0.006%
94	14.581	4193	4196	4199	rBV2	528	361	0.02%	0.003%
95	14.649	4215	4217	4220	rVB2	741	417	0.03%	0.003%
96	14.671	4221	4224	4226	rBV	548	389	0.02%	0.003%
97	14.778	4251	4257	4262	rBV3	786	1086	0.07%	0.008%
98	14.835	4271	4275	4277	rBV	596	487	0.03%	0.004%
99	15.575	4502	4505	4510	rBV4	1344	1242	0.08%	0.009%
100	15.665	4529	4533	4536	rBV3	906	942	0.06%	0.007%


Sum of corrected areas: 13562045

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030020.D
Acq On : 13 Mar 2019 10:55
Operator : JC/SP
Sample : K1734-15DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

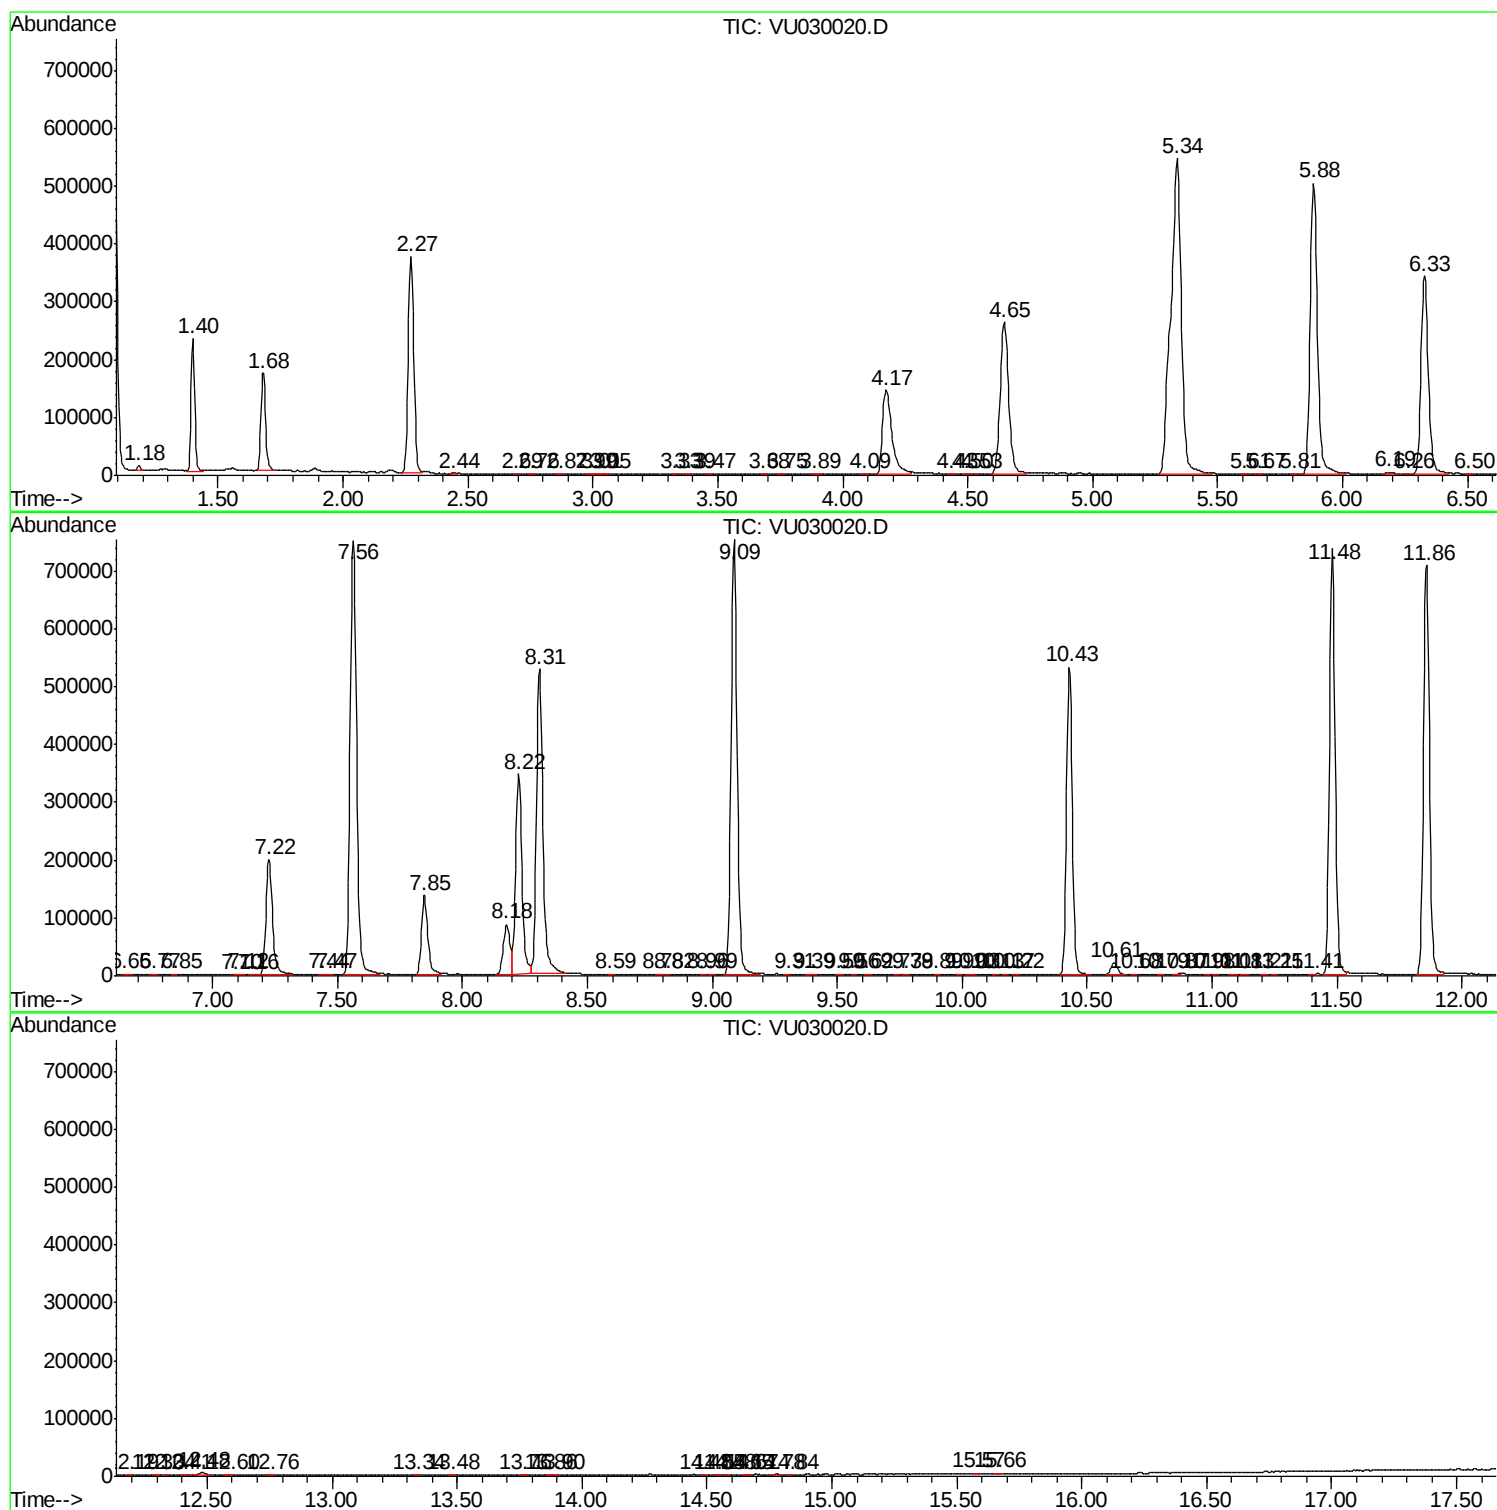

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030020.D
Acq On : 13 Mar 2019 10:55
Operator : JC/SP
Sample : K1734-15DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030020.D
Acq On : 13 Mar 2019 10:55
Operator : JC/SP
Sample : K1734-15DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc