

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030071.D
 Acq On : 14 Mar 2019 14:02
 Operator : JC/SP
 Sample : K1885-14DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	34	rVB	10293	8446	0.52%	0.060%
2	1.399	89	96	107	rBV	237238	241030	14.80%	1.719%
3	1.682	176	184	198	rVB	167859	210656	12.93%	1.502%
4	2.190	336	342	351	rBV8	3666	5528	0.34%	0.039%
5	2.273	356	368	381	rBV	371477	570845	35.05%	4.071%
6	2.434	415	418	421	rBV3	774	616	0.04%	0.004%
7	2.608	466	472	475	rVB2	598	474	0.03%	0.003%
8	2.698	494	500	501	rBV4	1461	1167	0.07%	0.008%
9	2.826	537	540	546	rVB2	758	792	0.05%	0.006%
10	3.145	629	639	644	rBV2	684	1027	0.06%	0.007%
11	3.177	644	649	651	rVV3	513	468	0.03%	0.003%
12	3.383	707	713	714	rBV2	438	430	0.03%	0.003%
13	3.505	747	751	753	rBV	501	383	0.02%	0.003%
14	3.624	782	788	791	rBV2	656	608	0.04%	0.004%
15	3.701	808	812	816	rBV	563	515	0.03%	0.004%
16	3.865	858	863	868	rBV2	366	399	0.02%	0.003%
17	3.945	883	888	890	rBV2	486	425	0.03%	0.003%
18	4.173	947	959	991	rBV	132219	345966	21.24%	2.467%
19	4.498	1056	1060	1063	rBV4	495	394	0.02%	0.003%
20	4.646	1089	1106	1138	rBV	244103	593762	36.45%	4.235%
21	5.061	1231	1235	1238	rBV3	678	486	0.03%	0.003%
22	5.106	1246	1249	1253	rBV2	443	430	0.03%	0.003%
23	5.337	1297	1321	1363	rBV2	528078	1525843	93.68%	10.882%
24	5.591	1396	1400	1403	rVB2	558	429	0.03%	0.003%
25	5.614	1403	1407	1411	rVB2	401	399	0.02%	0.003%
26	5.646	1411	1417	1421	rBV3	391	425	0.03%	0.003%
27	5.691	1426	1431	1434	rVB2	503	411	0.03%	0.003%
28	5.743	1439	1447	1448	rBV2	457	444	0.03%	0.003%
29	5.788	1458	1461	1465	rVB	488	378	0.02%	0.003%
30	5.884	1471	1491	1526	rBV	496071	1013811	62.24%	7.230%
31	6.154	1570	1575	1576	rBV2	462	411	0.03%	0.003%
32	6.180	1579	1583	1596	rVB8	2626	4222	0.26%	0.030%
33	6.279	1609	1614	1615	rBV3	559	419	0.03%	0.003%
34	6.328	1615	1629	1661	rBV	325903	660988	40.58%	4.714%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030071.D
 Acq On : 14 Mar 2019 14:02
 Operator : JC/SP
 Sample : K1885-14DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	6.566	1700	1703	1707	rVV2	577	564	0.03%	0.004%
36	6.595	1707	1712	1715	rVV2	510	529	0.03%	0.004%
37	6.646	1723	1728	1731	rBV2	552	449	0.03%	0.003%
38	6.685	1735	1740	1744	rBV	466	450	0.03%	0.003%
39	6.707	1744	1747	1750	rVB2	578	405	0.02%	0.003%
40	6.730	1750	1754	1756	rBV3	514	407	0.02%	0.003%
41	6.861	1790	1795	1797	rBV2	1105	945	0.06%	0.007%
42	7.225	1896	1908	1930	rBV	185076	340417	20.90%	2.428%
43	7.405	1961	1964	1967	rBV2	559	470	0.03%	0.003%
44	7.421	1967	1969	1974	rVB4	674	582	0.04%	0.004%
45	7.463	1974	1982	1983	rBV4	1174	1213	0.07%	0.009%
46	7.562	1999	2013	2048	rBV	703613	1273757	78.20%	9.084%
47	7.849	2090	2102	2127	rBV	125600	224427	13.78%	1.601%
48	8.080	2171	2174	2178	rBV4	468	396	0.02%	0.003%
49	8.109	2178	2183	2187	rVB4	633	628	0.04%	0.004%
50	8.177	2190	2204	2209	rBV	58588	105503	6.48%	0.752%
51	8.225	2209	2219	2235	rVV	939011	1628792	100.00%	11.616%
52	8.308	2235	2245	2271	rVB	469641	824950	50.65%	5.883%
53	8.678	2353	2360	2363	rBV3	613	720	0.04%	0.005%
54	8.742	2377	2380	2382	rBV3	598	374	0.02%	0.003%
55	8.762	2382	2386	2395	rVB4	677	928	0.06%	0.007%
56	8.804	2395	2399	2402	rBV2	540	447	0.03%	0.003%
57	8.858	2412	2416	2422	rBV3	737	692	0.04%	0.005%
58	9.086	2474	2487	2525	rBV	740314	1255794	77.10%	8.956%
59	9.308	2553	2556	2559	rBV3	950	600	0.04%	0.004%
60	9.643	2657	2660	2665	rVB3	567	388	0.02%	0.003%
61	9.787	2702	2705	2707	rBV2	589	370	0.02%	0.003%
62	9.987	2764	2767	2773	rBV	503	560	0.03%	0.004%
63	10.164	2817	2822	2826	rBV3	821	920	0.06%	0.007%
64	10.344	2874	2878	2881	rBV	559	411	0.03%	0.003%
65	10.427	2890	2904	2927	rBV	483404	780502	47.92%	5.566%
66	10.607	2949	2960	2977	rVB2	18752	32962	2.02%	0.235%
67	10.736	2994	3000	3007	rVB2	498	693	0.04%	0.005%
68	10.800	3015	3020	3023	rBV2	464	469	0.03%	0.003%
69	10.832	3023	3030	3031	rBV2	359	431	0.03%	0.003%
70	10.871	3036	3042	3044	rBV3	1212	1202	0.07%	0.009%
71	10.929	3057	3060	3063	rBV2	587	432	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030071.D
 Acq On : 14 Mar 2019 14:02
 Operator : JC/SP
 Sample : K1885-14DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1B3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	11.022	3084	3089	3094	rVB2	663	587	0.04%	0.004%
73	11.083	3105	3108	3111	rVB	558	380	0.02%	0.003%
74	11.106	3111	3115	3118	rBV2	602	491	0.03%	0.004%
75	11.125	3118	3121	3124	rVB3	572	407	0.02%	0.003%
76	11.151	3124	3129	3133	rBV2	486	488	0.03%	0.003%
77	11.418	3209	3212	3219	rVB5	1305	1313	0.08%	0.009%
78	11.482	3219	3232	3267	rBV	749523	1198109	73.56%	8.545%
79	11.858	3336	3349	3370	rBV	687274	1121448	68.85%	7.998%
80	12.260	3471	3474	3479	rVB4	653	496	0.03%	0.004%
81	12.421	3521	3524	3532	rBV2	697	659	0.04%	0.005%
82	12.479	3534	3542	3552	rVV	5416	8606	0.53%	0.061%
83	12.655	3591	3597	3598	rBV2	457	448	0.03%	0.003%
84	12.720	3614	3617	3623	rVB3	840	703	0.04%	0.005%
85	12.816	3642	3647	3650	rBV3	686	658	0.04%	0.005%
86	12.887	3664	3669	3673	rBV3	624	751	0.05%	0.005%
87	12.954	3687	3690	3692	rBV2	633	474	0.03%	0.003%
88	13.012	3703	3708	3712	rBV3	547	672	0.04%	0.005%
89	13.102	3733	3736	3739	rBV	468	370	0.02%	0.003%
90	13.417	3832	3834	3840	rVB3	703	716	0.04%	0.005%
91	13.659	3904	3909	3913	rVB2	548	548	0.03%	0.004%
92	13.688	3913	3918	3921	rBV2	597	542	0.03%	0.004%
93	13.710	3921	3925	3927	rBV	605	510	0.03%	0.004%
94	13.803	3947	3954	3957	rBV2	602	730	0.04%	0.005%
95	14.276	4098	4101	4109	rVB4	1813	2011	0.12%	0.014%
96	14.395	4135	4138	4140	rBV2	531	392	0.02%	0.003%
97	14.540	4179	4183	4186	rBV4	618	505	0.03%	0.004%
98	14.794	4256	4262	4264	rBV3	849	956	0.06%	0.007%
99	15.234	4397	4399	4402	rBV2	719	403	0.02%	0.003%
100	15.922	4610	4613	4615	rBV3	1220	786	0.05%	0.006%


Sum of corrected areas: 14021965

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030071.D
Acq On : 14 Mar 2019 14:02
Operator : JC/SP
Sample : K1885-14DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

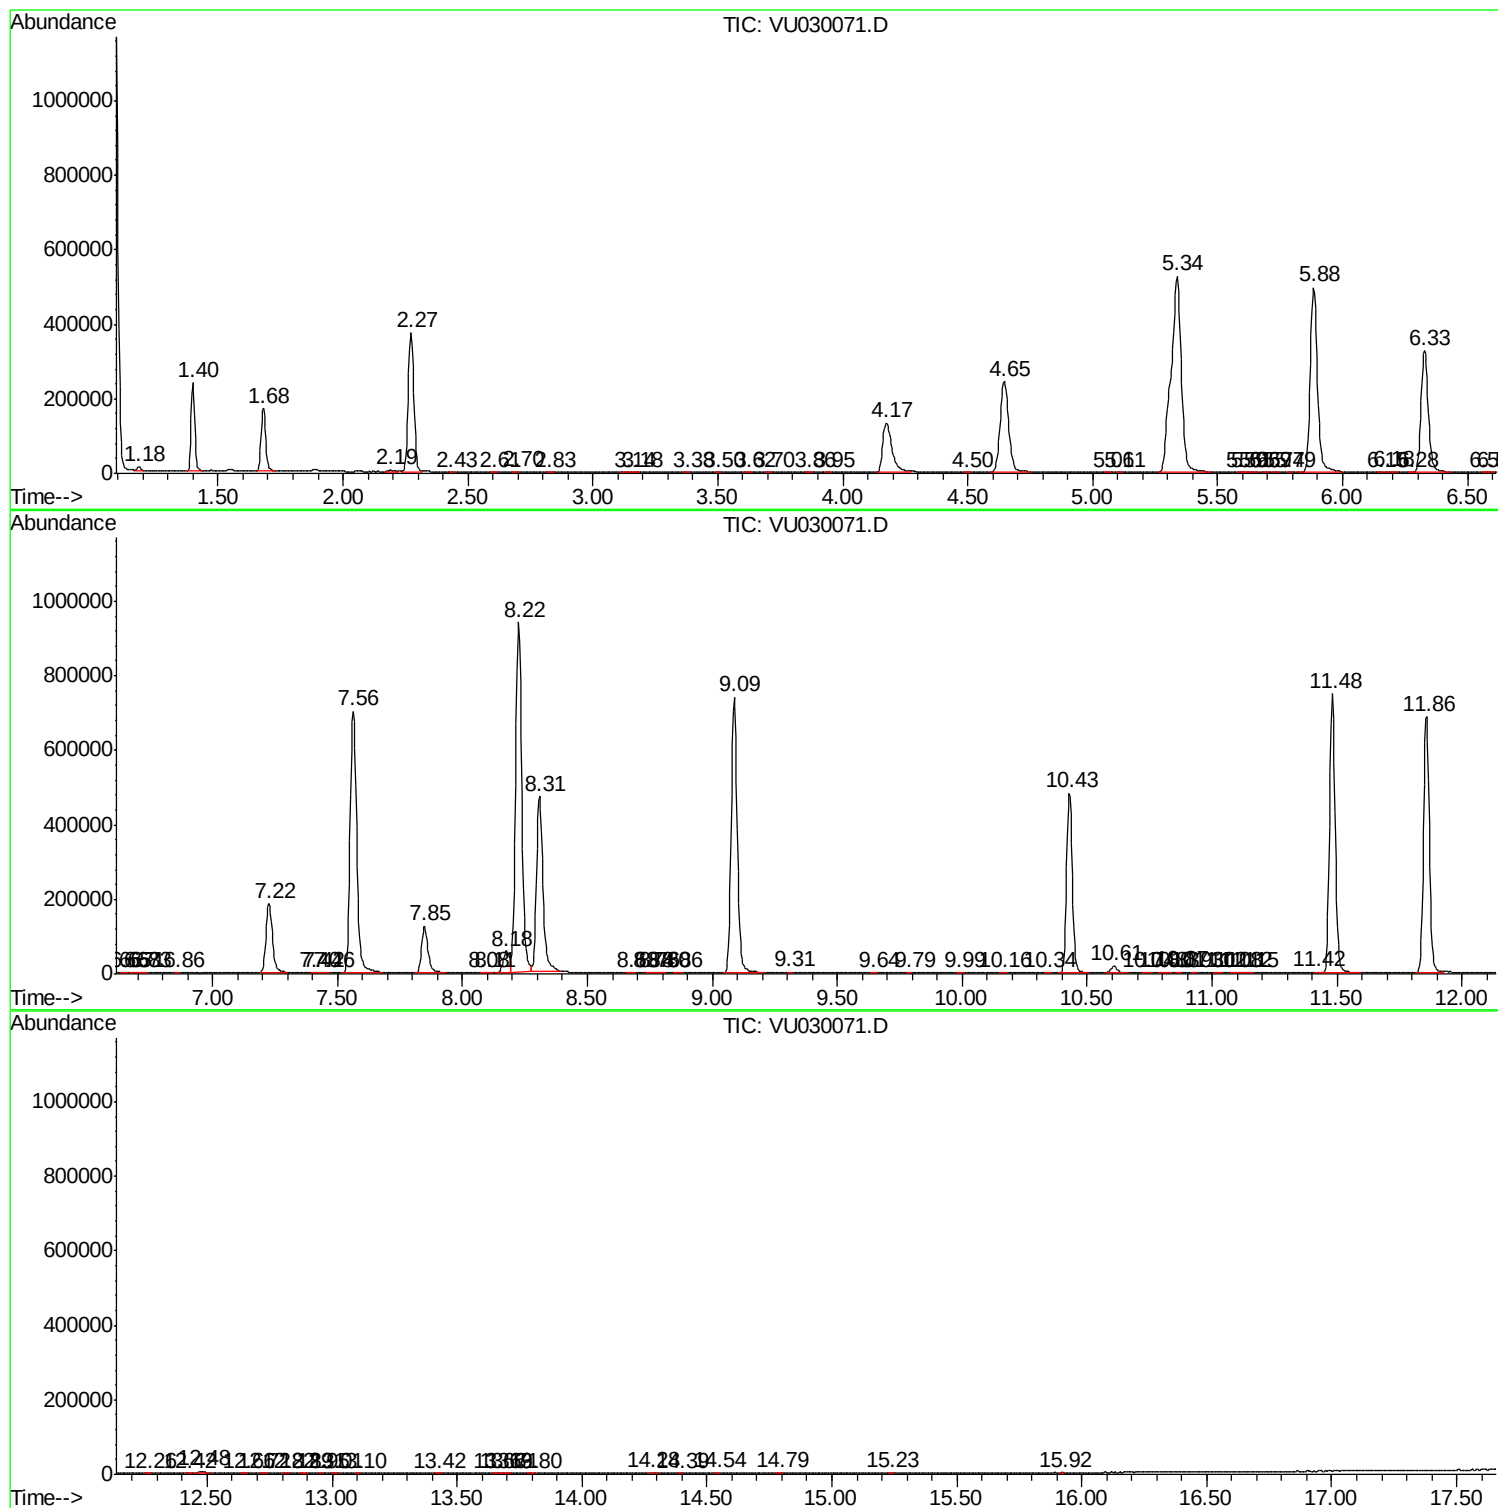

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030071.D
Acq On : 14 Mar 2019 14:02
Operator : JC/SP
Sample : K1885-14DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030071.D
Acq On : 14 Mar 2019 14:02
Operator : JC/SP
Sample : K1885-14DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1B3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc