

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030077.D
 Acq On : 14 Mar 2019 16:33
 Operator : JC/SP
 Sample : VU0315WBL04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK31

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	36	rVB2	11060	9689	0.56%	0.071%
2	1.399	89	96	107	rBV	255504	254777	14.83%	1.866%
3	1.678	175	183	196	rBV	184188	231600	13.48%	1.696%
4	2.270	356	367	380	rBV	408355	620935	36.14%	4.547%
5	2.476	427	431	438	rVB4	2244	2516	0.15%	0.018%
6	2.579	459	463	468	rVB3	563	610	0.04%	0.004%
7	2.624	474	477	481	rVV3	665	632	0.04%	0.005%
8	2.656	485	487	491	rVV2	649	472	0.03%	0.003%
9	2.704	493	502	516	rVB6	1818	3833	0.22%	0.028%
10	2.791	525	529	536	rBV3	387	400	0.02%	0.003%
11	2.981	582	588	589	rBV2	1417	1352	0.08%	0.010%
12	3.206	654	658	662	rVB2	572	507	0.03%	0.004%
13	3.296	682	686	689	rVB3	668	568	0.03%	0.004%
14	3.669	797	802	809	rVB3	556	607	0.04%	0.004%
15	3.752	824	828	831	rBV2	462	405	0.02%	0.003%
16	3.772	831	834	837	rVV2	698	527	0.03%	0.004%
17	3.791	837	840	845	rVB2	472	428	0.02%	0.003%
18	3.823	845	850	854	rBV3	452	439	0.03%	0.003%
19	3.897	866	873	876	rBV2	270	374	0.02%	0.003%
20	3.926	876	882	892	rVV2	782	1192	0.07%	0.009%
21	4.003	900	906	910	rBV3	650	622	0.04%	0.005%
22	4.174	946	959	995	rBV	149986	399873	23.28%	2.928%
23	4.530	1065	1070	1074	rVB3	457	456	0.03%	0.003%
24	4.643	1089	1105	1126	rBV	278012	665310	38.73%	4.872%
25	4.984	1206	1211	1213	rBV3	718	637	0.04%	0.005%
26	5.103	1239	1248	1252	rBV2	411	665	0.04%	0.005%
27	5.128	1252	1256	1260	rVV3	467	409	0.02%	0.003%
28	5.177	1265	1271	1273	rBV2	474	539	0.03%	0.004%
29	5.337	1296	1321	1350	rBV2	589354	1717952	100.00%	12.580%
30	5.627	1405	1411	1414	rVV3	524	648	0.04%	0.005%
31	5.656	1417	1420	1423	rBV2	902	538	0.03%	0.004%
32	5.672	1423	1425	1429	rVV2	610	391	0.02%	0.003%
33	5.762	1451	1453	1457	rVB2	599	489	0.03%	0.004%
34	5.788	1457	1461	1465	rVB2	583	514	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030077.D
 Acq On : 14 Mar 2019 16:33
 Operator : JC/SP
 Sample : VU0315WBL04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK31

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	5.884	1475	1491	1513	rBV	518107	1040240	60.55%	7.617%
36	6.173	1574	1581	1583	rBV4	2036	2478	0.14%	0.018%
37	6.225	1594	1597	1599	rBV3	601	377	0.02%	0.003%
38	6.328	1614	1629	1651	rBV	363866	748261	43.56%	5.479%
39	6.607	1713	1716	1721	rVB2	427	398	0.02%	0.003%
40	6.788	1768	1772	1778	rVB2	606	484	0.03%	0.004%
41	6.826	1778	1784	1788	rBV2	638	747	0.04%	0.005%
42	7.225	1891	1908	1939	rBV	200732	369391	21.50%	2.705%
43	7.357	1946	1949	1953	rVB2	700	457	0.03%	0.003%
44	7.463	1973	1982	1993	rBV6	3508	6497	0.38%	0.048%
45	7.562	1999	2013	2047	rBV	794429	1438032	83.71%	10.530%
46	7.845	2090	2101	2128	rBV	134469	244321	14.22%	1.789%
47	8.061	2164	2168	2171	rBV4	751	621	0.04%	0.005%
48	8.122	2184	2187	2191	rBV2	610	413	0.02%	0.003%
49	8.177	2192	2204	2215	rBV	29097	58352	3.40%	0.427%
50	8.308	2234	2245	2286	rVB	535420	941997	54.83%	6.898%
51	8.578	2324	2329	2335	rBV6	1204	1623	0.09%	0.012%
52	8.688	2359	2363	2367	rBV2	496	433	0.03%	0.003%
53	8.749	2378	2382	2387	rVB4	615	758	0.04%	0.006%
54	8.775	2387	2390	2393	rBV2	614	486	0.03%	0.004%
55	8.842	2406	2411	2414	rVB3	626	613	0.04%	0.004%
56	9.086	2473	2487	2515	rBV	773995	1306215	76.03%	9.565%
57	9.247	2532	2537	2540	rBV5	1235	1402	0.08%	0.010%
58	9.296	2547	2552	2555	rBV3	446	389	0.02%	0.003%
59	9.376	2568	2577	2589	rVB5	2053	4261	0.25%	0.031%
60	9.427	2589	2593	2598	rVB2	821	614	0.04%	0.004%
61	9.466	2601	2605	2611	rBV2	461	553	0.03%	0.004%
62	9.562	2633	2635	2643	rVB3	665	646	0.04%	0.005%
63	9.617	2647	2652	2655	rBV3	417	418	0.02%	0.003%
64	9.794	2699	2707	2711	rBV6	2191	3829	0.22%	0.028%
65	10.019	2771	2777	2781	rBV2	658	758	0.04%	0.006%
66	10.119	2803	2808	2811	rBV3	353	413	0.02%	0.003%
67	10.170	2817	2824	2834	rVB4	2339	4279	0.25%	0.031%
68	10.209	2834	2836	2840	rBV3	520	426	0.02%	0.003%
69	10.299	2859	2864	2866	rBV3	475	464	0.03%	0.003%
70	10.376	2884	2888	2891	rBV2	479	377	0.02%	0.003%
71	10.427	2892	2904	2922	rBV	546561	893845	52.03%	6.545%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030077.D
 Acq On : 14 Mar 2019 16:33
 Operator : JC/SP
 Sample : VU0315WBL04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK31

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	10.562	2942	2946	2949	rBV3	667	460	0.03%	0.003%
73	10.604	2951	2959	2974	rVB	9541	17171	1.00%	0.126%
74	10.710	2987	2992	2999	rBV3	486	594	0.03%	0.004%
75	10.955	3063	3068	3069	rBV2	541	414	0.02%	0.003%
76	11.048	3093	3097	3100	rBV2	637	421	0.02%	0.003%
77	11.209	3144	3147	3152	rVB2	663	571	0.03%	0.004%
78	11.421	3204	3213	3220	rBV4	4708	7955	0.46%	0.058%
79	11.482	3220	3232	3251	rBV	774935	1255190	73.06%	9.191%
80	11.858	3335	3349	3381	rBV	779064	1312554	76.40%	9.611%
81	12.167	3438	3445	3447	rBV4	797	789	0.05%	0.006%
82	12.215	3455	3460	3465	rBV4	574	616	0.04%	0.005%
83	12.276	3474	3479	3482	rBV3	1007	827	0.05%	0.006%
84	12.311	3488	3490	3495	rVV2	368	375	0.02%	0.003%
85	12.475	3533	3541	3550	rBV4	2061	3528	0.21%	0.026%
86	12.607	3577	3582	3586	rBV2	668	590	0.03%	0.004%
87	12.662	3594	3599	3603	rBV5	680	803	0.05%	0.006%
88	12.893	3664	3671	3682	rBV5	4431	7931	0.46%	0.058%
89	13.061	3717	3723	3727	rBV2	829	1073	0.06%	0.008%
90	13.109	3735	3738	3743	rBV2	542	434	0.03%	0.003%
91	13.321	3800	3804	3809	rBV2	450	557	0.03%	0.004%
92	13.405	3826	3830	3834	rVB2	860	662	0.04%	0.005%
93	13.511	3855	3863	3878	rBV4	7039	14435	0.84%	0.106%
94	13.697	3917	3921	3924	rBV2	500	455	0.03%	0.003%
95	13.755	3931	3939	3948	rBV2	6442	13697	0.80%	0.100%
96	13.996	4005	4014	4028	rBV4	7619	14801	0.86%	0.108%
97	14.131	4052	4056	4060	rVB2	655	492	0.03%	0.004%
98	14.212	4076	4081	4084	rBV3	792	766	0.04%	0.006%
99	14.273	4096	4100	4101	rBV2	1043	749	0.04%	0.005%
100	14.829	4270	4273	4277	rBV2	787	694	0.04%	0.005%


Sum of corrected areas: 13656378

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030077.D
Acq On : 14 Mar 2019 16:33
Operator : JC/SP
Sample : VU0315WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK31

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

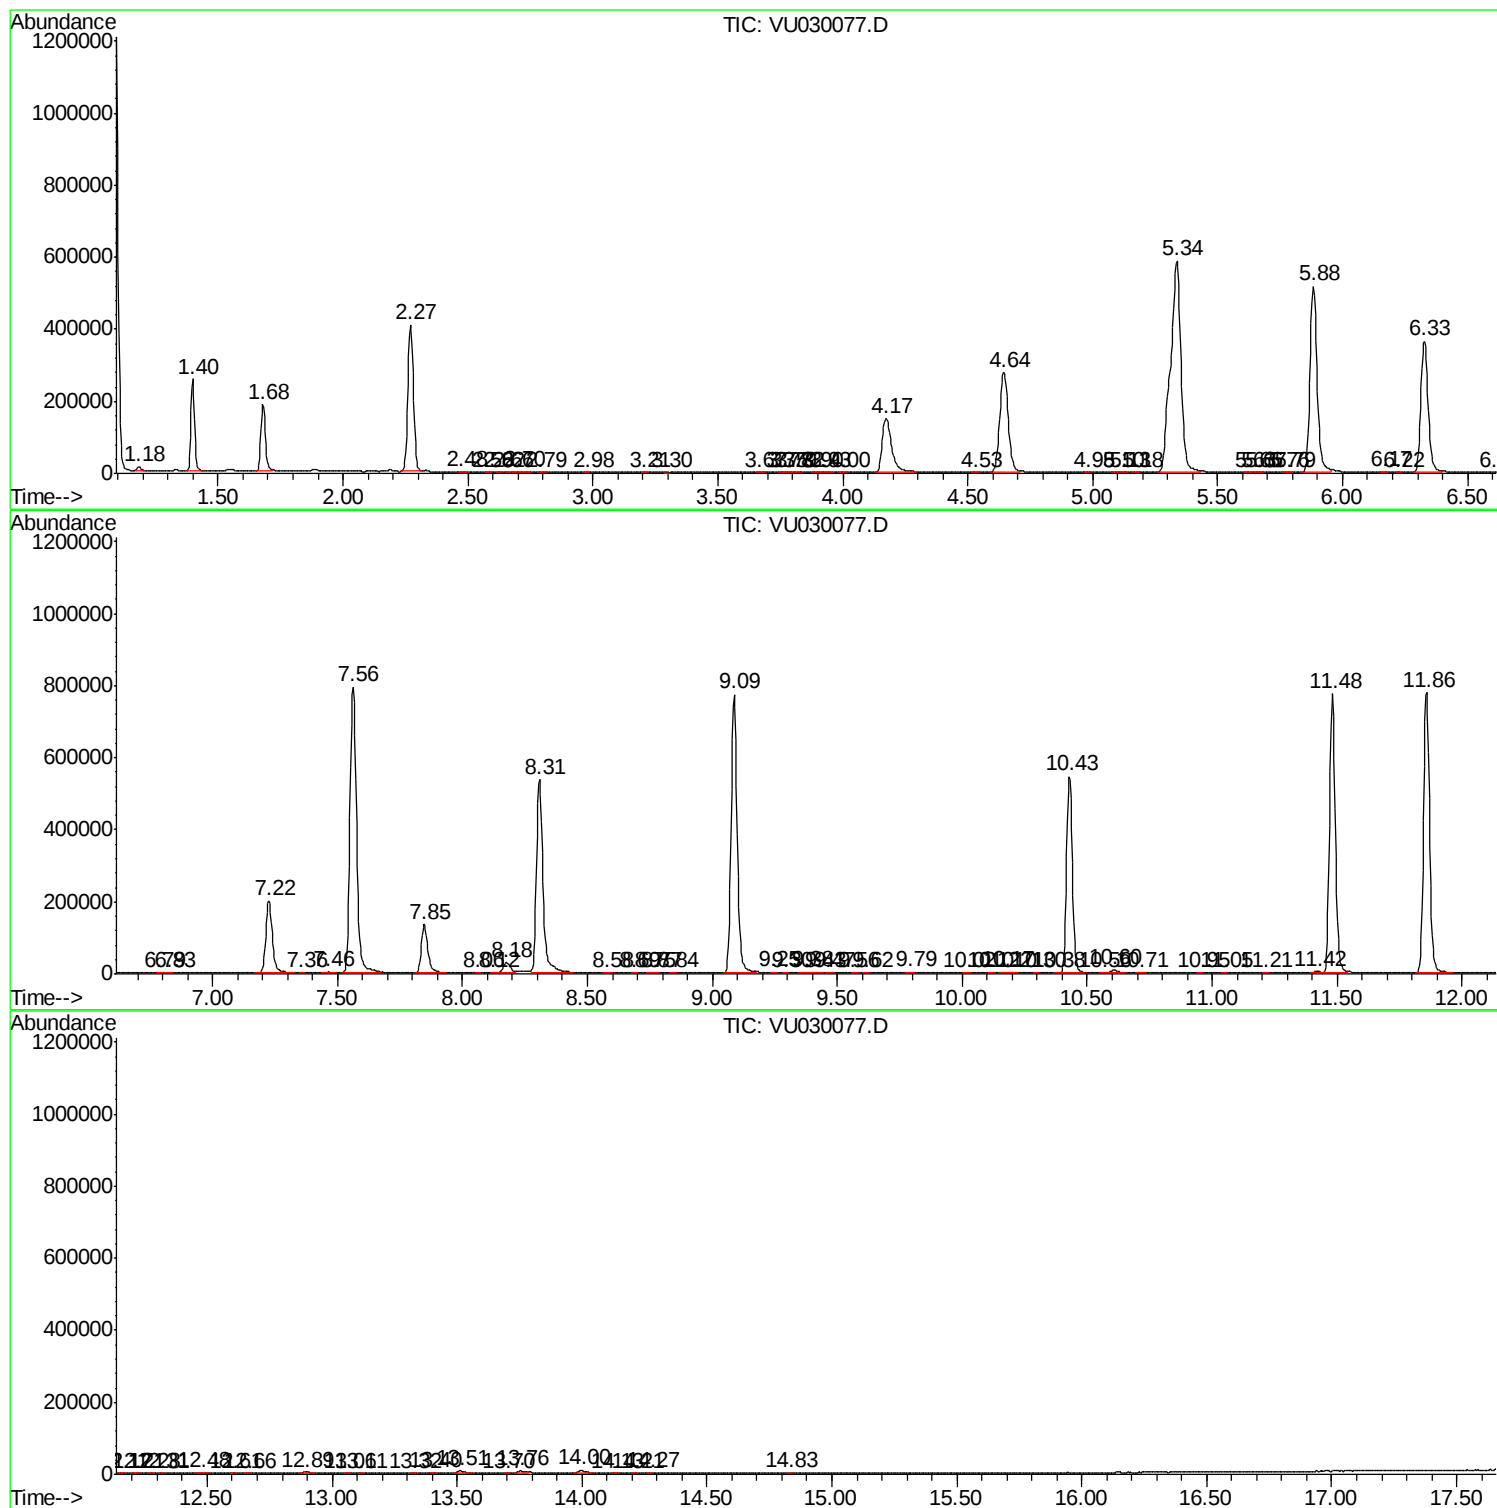

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030077.D
Acq On : 14 Mar 2019 16:33
Operator : JC/SP
Sample : VU0315WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK31

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU031519\
Data File : VU030077.D
Acq On : 14 Mar 2019 16:33
Operator : JC/SP
Sample : VU0315WBL04
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
VBLK31

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc