

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030083.D
 Acq On : 14 Mar 2019 18:52
 Operator : JC/SP
 Sample : K1859-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BR0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.184	24	29	35	rVB2	10339	9530	0.47%	0.069%
2	1.399	89	96	107	rBV	165287	164404	8.10%	1.184%
3	1.679	175	183	199	rBV	137177	179399	8.83%	1.292%
4	2.190	335	342	348	rBV5	3831	5196	0.26%	0.037%
5	2.270	357	367	380	rBV	296514	452090	22.26%	3.256%
6	2.444	412	421	438	rBV	17631	32967	1.62%	0.237%
7	2.505	438	440	444	rVB3	782	525	0.03%	0.004%
8	2.701	494	501	508	rBV6	1382	2279	0.11%	0.016%
9	2.743	512	514	518	rVB2	600	387	0.02%	0.003%
10	3.029	600	603	608	rBV	726	636	0.03%	0.005%
11	3.093	620	623	627	rVB3	565	417	0.02%	0.003%
12	3.151	638	641	643	rBV2	502	343	0.02%	0.002%
13	3.193	650	654	662	rBV	679	831	0.04%	0.006%
14	3.296	681	686	689	rBV4	590	521	0.03%	0.004%
15	3.386	711	714	723	rVB3	482	649	0.03%	0.005%
16	3.434	723	729	734	rBV2	437	593	0.03%	0.004%
17	3.711	810	815	818	rVB2	354	326	0.02%	0.002%
18	3.785	831	838	841	rBV	405	439	0.02%	0.003%
19	3.839	849	855	859	rBV2	372	444	0.02%	0.003%
20	4.106	935	938	942	rVB	666	482	0.02%	0.003%
21	4.174	947	959	997	rBV	148182	395923	19.50%	2.852%
22	4.646	1088	1106	1128	rBV	243023	582582	28.69%	4.196%
23	4.920	1189	1191	1193	rBV2	637	378	0.02%	0.003%
24	4.936	1193	1196	1199	rVB3	652	457	0.02%	0.003%
25	4.952	1199	1201	1204	rBV3	562	385	0.02%	0.003%
26	4.987	1209	1212	1215	rBV3	877	699	0.03%	0.005%
27	5.113	1248	1251	1253	rBV3	533	387	0.02%	0.003%
28	5.193	1273	1276	1280	rBV2	431	405	0.02%	0.003%
29	5.338	1295	1321	1332	rBV2	490544	1454187	71.61%	10.474%
30	5.518	1374	1377	1383	rVB4	591	602	0.03%	0.004%
31	5.592	1392	1400	1405	rVB3	578	721	0.04%	0.005%
32	5.743	1443	1447	1450	rBV2	454	452	0.02%	0.003%
33	5.884	1476	1491	1533	rBV	490341	1004085	49.44%	7.232%
34	6.187	1575	1585	1591	rBV7	1876	3209	0.16%	0.023%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030083.D
 Acq On : 14 Mar 2019 18:52
 Operator : JC/SP
 Sample : K1859-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BR0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

35	6.328	1615	1629	1667	rBV	321081	656845	32.34%	4.731%
36	6.495	1679	1681	1685	rVB2	552	364	0.02%	0.003%
37	6.576	1700	1706	1710	rBV2	397	468	0.02%	0.003%
38	6.624	1716	1721	1724	rVB	608	451	0.02%	0.003%
39	6.643	1724	1727	1734	rBV2	477	555	0.03%	0.004%
40	6.871	1791	1798	1801	rBV3	885	1101	0.05%	0.008%
41	6.984	1829	1833	1836	rVB2	432	341	0.02%	0.002%
42	7.109	1869	1872	1875	rBV2	616	540	0.03%	0.004%
43	7.164	1886	1889	1894	rBV2	414	415	0.02%	0.003%
44	7.225	1894	1908	1932	rBV	179587	336728	16.58%	2.425%
45	7.334	1939	1942	1948	rVB4	774	747	0.04%	0.005%
46	7.367	1948	1952	1959	rVB4	627	634	0.03%	0.005%
47	7.479	1982	1987	1997	rVB5	926	1350	0.07%	0.010%
48	7.563	1997	2013	2054	rBV	651751	1193332	58.76%	8.595%
49	7.846	2090	2101	2133	rVV	128068	227944	11.22%	1.642%
50	8.061	2166	2168	2171	rVB2	777	420	0.02%	0.003%
51	8.177	2186	2204	2218	rBV2	45950	90963	4.48%	0.655%
52	8.309	2234	2245	2276	rVB	512034	887835	43.72%	6.395%
53	8.662	2350	2355	2356	rBV2	552	363	0.02%	0.003%
54	8.714	2369	2371	2373	rVV2	616	327	0.02%	0.002%
55	8.788	2390	2394	2396	rBV	471	353	0.02%	0.003%
56	8.958	2440	2447	2451	rBV3	564	817	0.04%	0.006%
57	9.087	2472	2487	2491	rBV	751695	1179997	58.10%	8.499%
58	9.354	2566	2570	2572	rBV2	460	343	0.02%	0.002%
59	9.379	2572	2578	2581	rBV5	787	983	0.05%	0.007%
60	9.415	2587	2589	2592	rBV	444	376	0.02%	0.003%
61	9.453	2596	2601	2606	rVB3	705	744	0.04%	0.005%
62	9.579	2638	2640	2644	rVB	411	320	0.02%	0.002%
63	9.730	2683	2687	2691	rBV2	579	506	0.02%	0.004%
64	9.775	2698	2701	2703	rBV	656	431	0.02%	0.003%
65	9.923	2742	2747	2751	rBV	331	402	0.02%	0.003%
66	9.968	2756	2761	2763	rVB2	394	326	0.02%	0.002%
67	10.042	2781	2784	2789	rVB2	611	566	0.03%	0.004%
68	10.093	2793	2800	2804	rBV3	719	878	0.04%	0.006%
69	10.167	2816	2823	2828	rBV5	1287	1729	0.09%	0.012%
70	10.366	2882	2885	2890	rVB	474	345	0.02%	0.002%
71	10.428	2891	2904	2932	rBV	520741	849030	41.81%	6.115%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030083.D
 Acq On : 14 Mar 2019 18:52
 Operator : JC/SP
 Sample : K1859-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BR0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis

72	10.604	2948	2959	2973	rBV2	16976	29084	1.43%	0.209%
73	10.675	2978	2981	2984	rVB	665	382	0.02%	0.003%
74	10.878	3039	3044	3048	rBV3	1057	1079	0.05%	0.008%
75	11.083	3105	3108	3112	rBV4	637	665	0.03%	0.005%
76	11.222	3146	3151	3156	rBV2	453	504	0.02%	0.004%
77	11.418	3197	3212	3220	rBV	44780	71227	3.51%	0.513%
78	11.482	3220	3232	3263	rVB2	806663	1843008	90.75%	13.274%
79	11.862	3333	3350	3378	rBV3	868634	2030805	100.00%	14.627%
80	12.090	3418	3421	3426	rBV4	733	761	0.04%	0.005%
81	12.193	3449	3453	3461	rVB5	678	760	0.04%	0.005%
82	12.292	3479	3484	3489	rVV4	708	658	0.03%	0.005%
83	12.479	3533	3542	3554	rVB2	6505	10237	0.50%	0.074%
84	12.836	3650	3653	3658	rVB3	590	504	0.02%	0.004%
85	13.013	3704	3708	3713	rBV3	445	431	0.02%	0.003%
86	13.080	3726	3729	3734	rBV3	490	415	0.02%	0.003%
87	13.109	3734	3738	3740	rBV2	578	423	0.02%	0.003%
88	13.173	3755	3758	3765	rVB2	584	599	0.03%	0.004%
89	13.209	3766	3769	3775	rBV2	454	511	0.03%	0.004%
90	13.321	3800	3804	3806	rBV	519	441	0.02%	0.003%
91	13.363	3813	3817	3821	rBV2	540	550	0.03%	0.004%
92	13.450	3841	3844	3850	rVB3	463	432	0.02%	0.003%
93	13.505	3851	3861	3886	rBV	54498	113107	5.57%	0.815%
94	13.730	3928	3931	3934	rBV2	619	524	0.03%	0.004%
95	13.858	3969	3971	3974	rBV	506	356	0.02%	0.003%
96	13.993	4003	4013	4032	rBV3	14576	33410	1.65%	0.241%
97	14.144	4056	4060	4064	rBV	733	691	0.03%	0.005%
98	14.273	4093	4100	4111	rBV2	2628	4428	0.22%	0.032%
99	14.575	4191	4194	4196	rBV	556	362	0.02%	0.003%
100	15.569	4499	4503	4507	rBV2	991	1027	0.05%	0.007%


Sum of corrected areas: 13884180

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030083.D
Acq On : 14 Mar 2019 18:52
Operator : JC/SP
Sample : K1859-05DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0BR0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

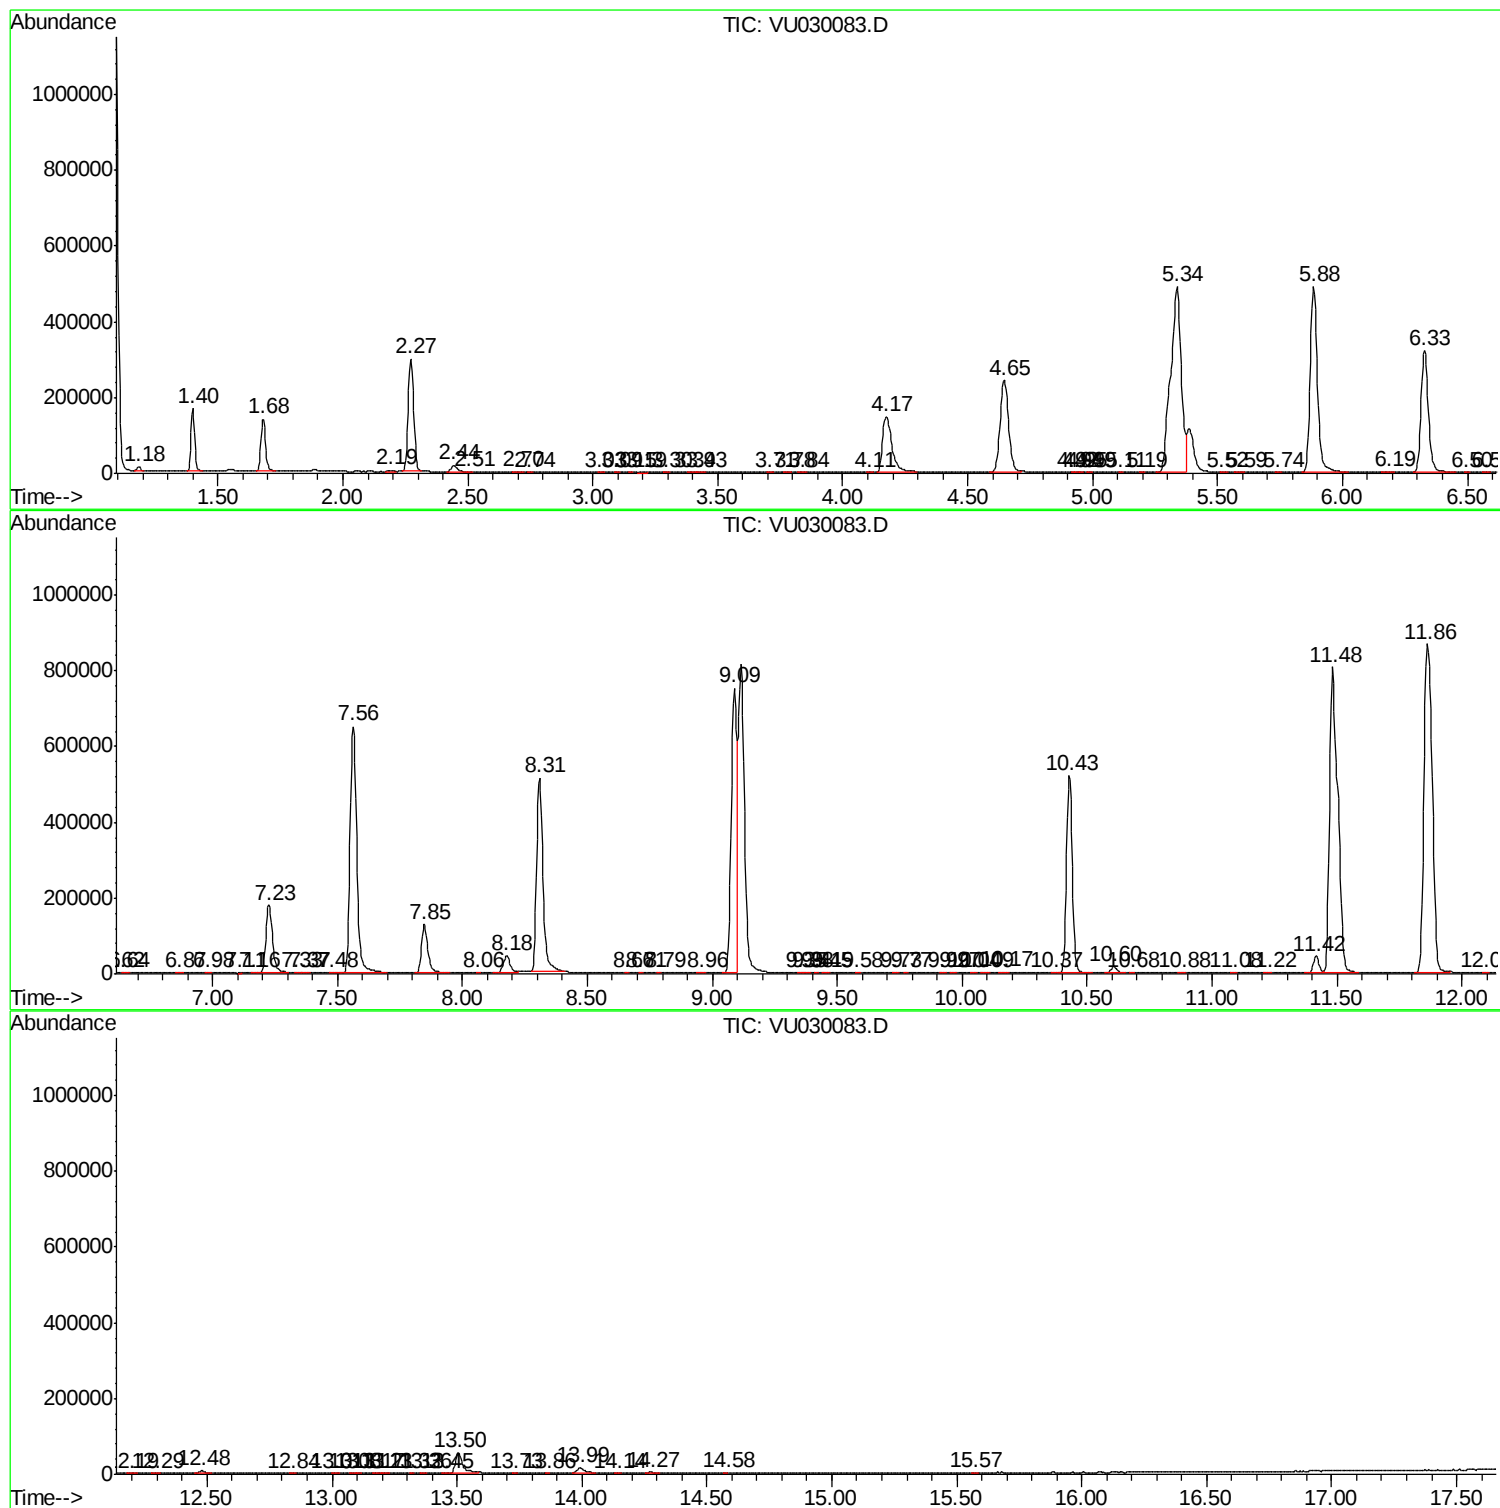

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
Data File : VU030083.D
Acq On : 14 Mar 2019 18:52
Operator : JC/SP
Sample : K1859-05DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BR0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU031519\
Data File : VU030083.D
Acq On : 14 Mar 2019 18:52
Operator : JC/SP
Sample : K1859-05DL 500X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0BR0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM031319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc