


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030014.D
 Acq On : 13 Mar 2019 08:25
 Operator : JC/SP
 Sample : BFB32
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB32

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis
 Last Update : Sat Mar 16 00:02:21 2019

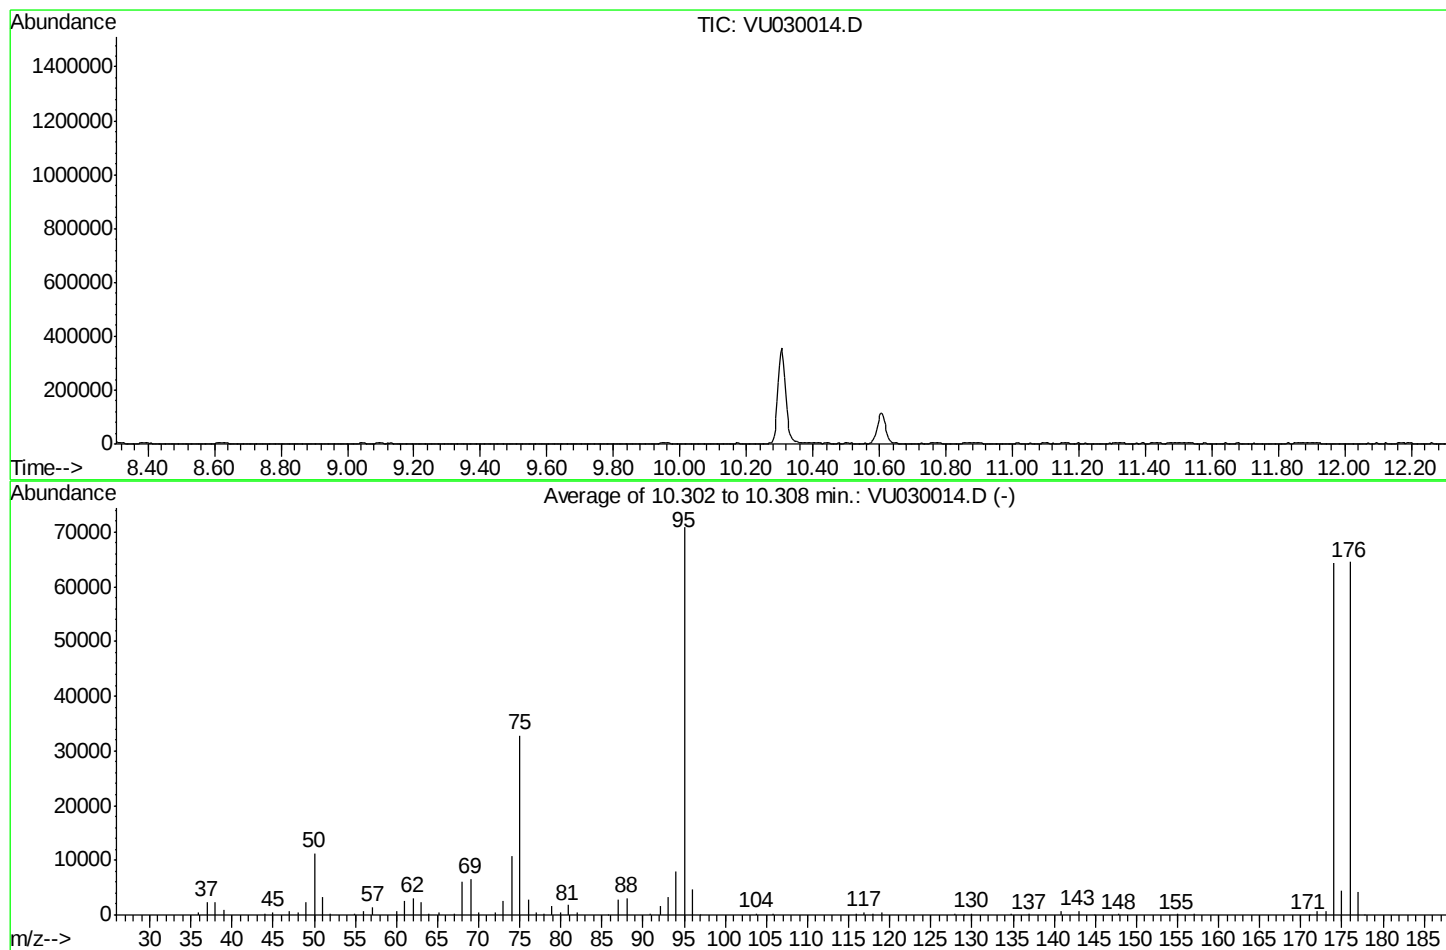

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	11334	PASS
75	95	30	80	46.3	32832	PASS
95	95	100	100	100.0	70858	PASS
96	95	5	9	6.8	4785	PASS
173	174	0.00	2	0.9	607	PASS
174	95	50	120	90.9	64429	PASS
175	174	5	9	7.0	4514	PASS
176	174	95	101	100.2	64562	PASS
177	176	5	9	6.6	4247	PASS

Scan 2853 (10.263 min): VU030014.D
BFB32

m/z	Abundance
35.90	378.0
38.00	131.0
39.90	1519.0
44.00	339.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	850.0
37.00	2460.0
38.00	2354.0
39.00	1018.0
40.00	1454.0
44.00	614.0
45.00	509.0
47.00	713.0
48.00	440.0
49.00	2220.0
50.00	11310.0
51.00	3290.0
51.90	141.0
54.90	147.0
56.00	660.0
57.10	1387.0
60.00	681.0
61.00	2591.0
62.00	3056.0
63.00	2286.0
63.90	301.0
65.10	439.0
67.10	261.0
68.00	5856.0
69.00	6504.0
70.00	527.0
72.00	347.0
73.00	2703.0
74.00	10918.0
75.00	32128.0
76.00	2991.0
77.00	473.0
78.00	288.0
78.90	1650.0
79.90	554.0
80.90	1835.0
81.90	525.0
85.80	134.0
87.10	2734.0
88.00	3259.0
90.80	265.0
92.10	1693.0
93.00	3213.0
94.00	7547.0
95.00	69008.0
96.00	4585.0
97.00	101.0
104.00	174.0
105.90	206.0
115.90	216.0
116.90	493.0
118.00	218.0
119.00	441.0
127.90	206.0
129.00	149.0
130.00	239.0
134.80	129.0
137.00	150.0
140.90	613.0
143.00	729.0
144.80	161.0
147.90	151.0
154.90	155.0
157.00	142.0
171.00	119.0
172.00	693.0
173.00	639.0
174.00	62440.0
175.00	4232.0
176.00	61584.0
177.00	4001.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	802.0
37.00	2469.0
38.00	2459.0
39.00	1102.0
39.90	1464.0
44.00	648.0
45.00	517.0
47.00	757.0
48.00	435.0
49.00	2422.0
50.00	11700.0
51.00	3462.0
51.90	167.0
54.90	191.0
56.00	751.0
57.10	1534.0
60.00	737.0
61.10	2646.0
62.10	3259.0
63.00	2547.0
63.90	301.0
65.10	453.0
67.10	281.0
68.00	6232.0
69.00	6738.0
70.00	555.0
72.00	414.0
73.00	2675.0
74.00	11206.0
75.00	33904.0
76.00	2959.0
76.90	508.0
78.00	329.0
78.90	1780.0
79.90	549.0
80.90	1855.0
81.90	526.0
85.80	106.0
87.00	2850.0
88.00	3154.0
90.80	317.0
92.10	1624.0
93.00	3385.0
94.00	8090.0
95.00	72920.0
96.00	4885.0
97.00	104.0
103.80	252.0
105.90	194.0
115.90	241.0
116.90	490.0
117.90	232.0
119.00	408.0
127.80	244.0
129.00	113.0
129.90	249.0
134.80	153.0
137.00	166.0
140.90	652.0
143.00	790.0
144.90	125.0
147.90	170.0
154.90	133.0
157.00	132.0
171.00	100.0
172.00	728.0
173.10	612.0
174.00	66088.0
175.00	4629.0
176.00	66856.0
177.00	4402.0
177.70	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	736.0
37.00	2310.0
38.00	2427.0
39.00	1046.0
39.90	1498.0
44.00	633.0
45.00	514.0
47.00	664.0
48.00	366.0
49.00	2312.0
50.00	10992.0
51.00	3236.0
51.90	211.0
54.90	192.0
56.00	818.0
57.10	1572.0
60.00	663.0
61.00	2491.0
62.10	3053.0
63.00	2409.0
63.90	281.0
65.10	432.0
67.00	233.0
68.00	5998.0
69.00	6514.0
70.00	487.0
72.00	413.0
73.00	2563.0
74.00	10486.0
75.00	32464.0
76.00	2619.0
76.90	446.0
78.00	429.0
78.90	1766.0
79.90	502.0
80.90	1719.0
82.00	531.0
86.90	2680.0
88.00	2741.0
90.80	272.0
92.10	1427.0
93.00	3058.0
94.00	7980.0
95.00	70648.0
96.00	4885.0
97.00	117.0
103.80	316.0
105.80	192.0
115.90	231.0
116.90	474.0
117.90	221.0
119.00	328.0
127.90	249.0
129.90	265.0
134.80	163.0
137.00	148.0
140.90	686.0
143.00	805.0
147.90	153.0
155.00	124.0
156.90	111.0
172.00	677.0
173.10	572.0
174.00	64760.0
175.00	4682.0
176.00	65248.0
177.00	4339.0
177.70	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32