


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU031519\
 Data File : VU030058.D
 Acq On : 14 Mar 2019 08:54
 Operator : JC/SP
 Sample : BFB33
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB33

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM031319WMA.M
 Title : VOC Analysis
 Last Update : Sat Mar 16 00:02:21 2019

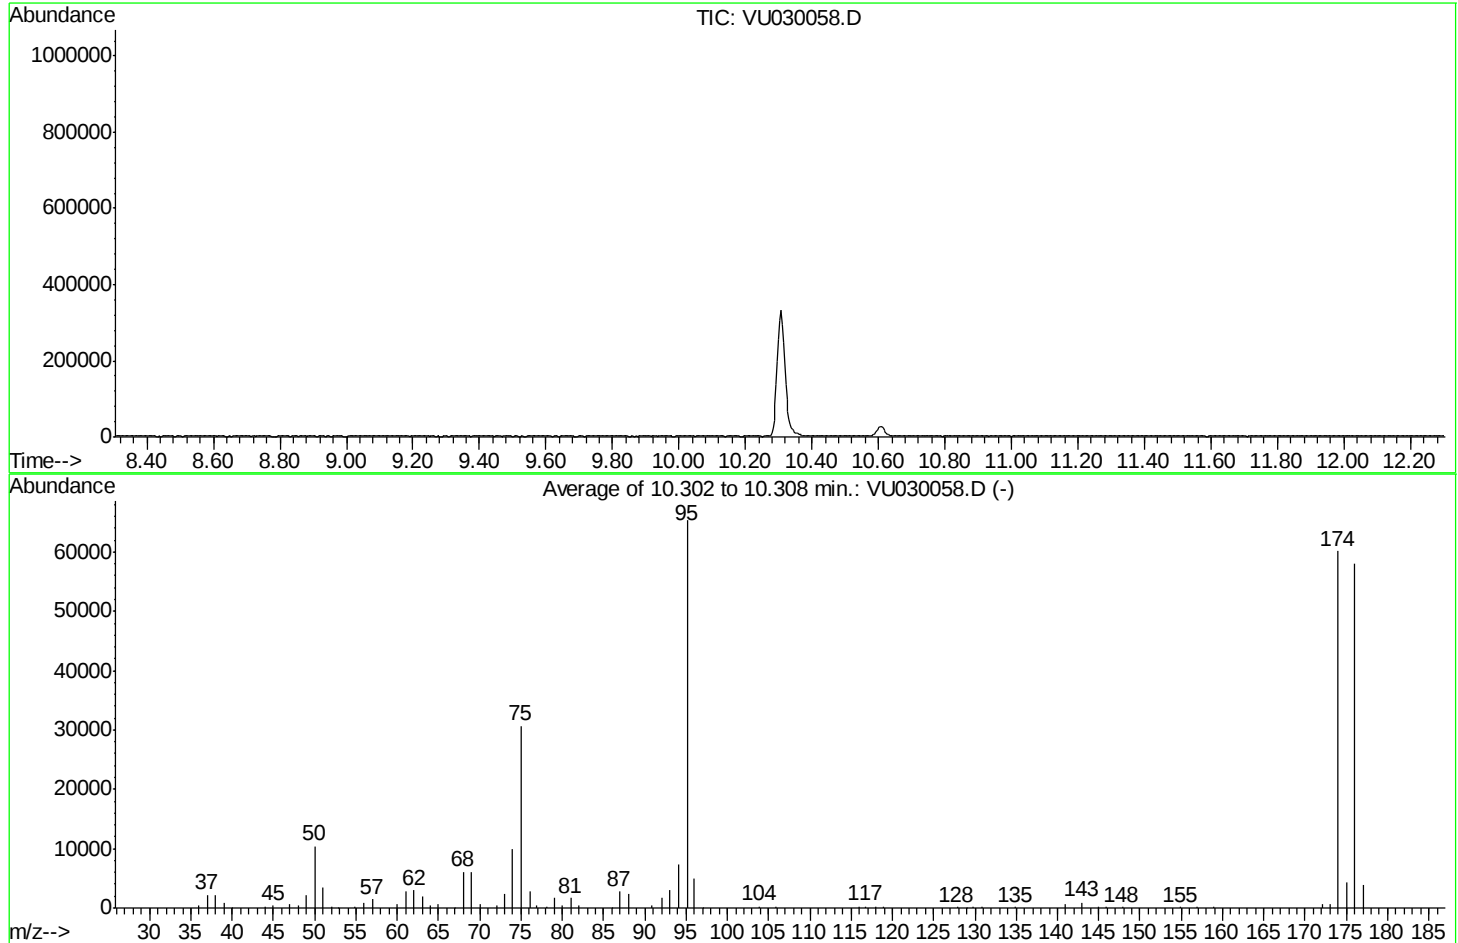

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	10446	PASS
75	95	30	80	47.0	30696	PASS
95	95	100	100	100.0	65330	PASS
96	95	5	9	7.6	4950	PASS
173	174	0.00	2	1.1	655	PASS
174	95	50	120	92.0	60085	PASS
175	174	5	9	7.1	4262	PASS
176	174	95	101	96.6	58050	PASS
177	176	5	9	6.7	3897	PASS

m/z	Abundance
39.90	1458.0
43.90	363.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.90	476.0
37.00	2100.0
38.00	2055.0
39.00	959.0
40.00	1636.0
44.00	617.0
45.00	377.0
47.00	641.0
47.90	351.0
49.00	2079.0
50.00	10256.0
51.00	3277.0
52.00	150.0
54.90	167.0
56.00	924.0
57.00	1322.0
60.00	509.0
61.00	2660.0
62.00	2842.0
63.10	1896.0
64.00	408.0
65.00	494.0
68.00	6023.0
69.00	5780.0
70.00	544.0
72.00	323.0
73.00	2430.0
74.00	9333.0
75.00	29480.0
76.10	2632.0
76.90	480.0
78.10	230.0
79.00	1594.0
80.00	443.0
81.00	1695.0
81.90	422.0
86.00	169.0
86.90	2424.0
88.00	2199.0
90.90	272.0
92.00	1499.0
93.00	2674.0
94.10	7228.0
95.10	62464.0
96.00	4775.0
103.90	240.0
105.90	254.0
115.90	159.0
116.80	319.0
118.00	228.0
118.90	311.0
127.80	200.0
129.70	145.0
131.00	136.0
134.90	125.0
140.90	594.0
143.00	946.0
144.90	134.0
145.90	129.0
147.90	130.0
154.90	184.0
157.00	135.0
158.90	103.0
172.00	656.0
173.00	609.0
174.00	56656.0
175.00	4040.0
176.00	53136.0
177.00	3898.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.90	469.0
37.00	2349.0
38.00	2248.0
39.00	948.0
40.00	1534.0
44.00	623.0
45.00	350.0
47.00	701.0
48.00	384.0
49.00	2188.0
50.00	10916.0
51.00	3473.0
52.10	170.0
52.80	108.0
54.90	178.0
56.00	853.0
57.00	1498.0
60.00	605.0
61.00	2858.0
62.00	3115.0
63.10	2110.0
64.00	446.0
65.00	568.0
67.00	144.0
68.00	6312.0
69.00	6174.0
70.00	571.0
72.00	387.0
73.00	2482.0
74.00	10321.0
75.00	31816.0
76.10	2813.0
77.00	518.0
78.00	214.0
79.00	1690.0
80.00	491.0
81.00	1704.0
82.00	489.0
86.90	2794.0
88.00	2344.0
90.90	348.0
92.00	1765.0
93.00	3037.0
94.10	7560.0
95.10	67152.0
96.00	5142.0
103.90	327.0
105.80	301.0
115.90	249.0
116.80	328.0
117.90	227.0
119.00	335.0
127.80	218.0
129.00	100.0
129.80	169.0
130.90	136.0
134.90	115.0
140.90	658.0
143.00	974.0
144.90	149.0
145.80	142.0
147.90	144.0
155.00	201.0
157.00	143.0
158.90	135.0
172.00	700.0
173.00	663.0
174.00	61936.0
175.00	4428.0
176.00	59584.0
177.00	4046.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.90	405.0
37.00	2311.0
38.00	2228.0
39.00	877.0
40.00	1460.0
44.00	608.0
45.00	333.0
47.00	723.0
48.00	386.0
49.00	2153.0
50.00	10167.0
51.00	3358.0
52.00	140.0
54.80	166.0
56.00	732.0
57.00	1456.0
60.00	651.0
61.00	2673.0
62.00	2899.0
63.10	2105.0
64.00	393.0
65.00	584.0
67.00	164.0
68.00	5888.0
69.00	5977.0
70.00	533.0
72.00	415.0
73.00	2402.0
74.00	10181.0
75.00	30792.0
76.10	2920.0
77.00	517.0
78.00	170.0
79.00	1625.0
80.10	485.0
81.00	1664.0
81.90	474.0
87.00	2911.0
88.00	2514.0
90.90	377.0
92.00	1796.0
93.00	3068.0
94.10	7251.0
95.10	66376.0
96.00	4934.0
97.10	108.0
103.90	347.0
105.80	322.0
115.90	261.0
116.80	338.0
117.90	182.0
119.00	325.0
127.90	212.0
129.00	136.0
129.90	201.0
130.80	143.0
135.00	126.0
140.90	693.0
143.00	884.0
144.90	148.0
145.90	130.0
147.90	134.0
155.00	176.0
156.90	122.0
158.90	134.0
172.10	692.0
173.00	695.0
174.00	61664.0
175.00	4319.0
176.00	61432.0
177.00	3747.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33