

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031521\
 Data File : VU042673.D
 Acq On : 15 Mar 2021 18:56
 Operator : SY/MD
 Sample : M1676-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Quant Time: Mar 16 01:40:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 16 01:32:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	75120	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	74721	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.819	152	34602	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	20224	4.04	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.80%
7) Chloroethane-d5	1.919	69	18581	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.00%
11) 1,1-Dichloroethene-d2	2.575	63	35680	3.15	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.00%
20) 2-Butanone-d5	4.649	46	78752	47.90	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.80%
24) Chloroform-d	5.073	84	48971	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.713	65	32373	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.20%
32) Benzene-d6	5.735	84	87520	4.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.60%
36) 1,2-Dichloropropane-d6	6.700	67	29726	5.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.60%
41) Toluene-d8	7.906	98	82100	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.80%
43) trans-1,3-Dichloroprop...	8.189	79	11429	4.14	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.80%
46) 2-Hexanone-d5	8.645	63	60495	45.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.52%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	25596	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	12.201	152	31698	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%
Target Compounds						Qvalue
16) Methylene chloride	3.054	84	1773	0.28	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031521\
Data File : VU042673.D
Acq On : 15 Mar 2021 18:56
Operator : SY/MD
Sample : M1676-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Time: Mar 16 01:40:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Mar 16 01:32:07 2021
Response via : Initial Calibration

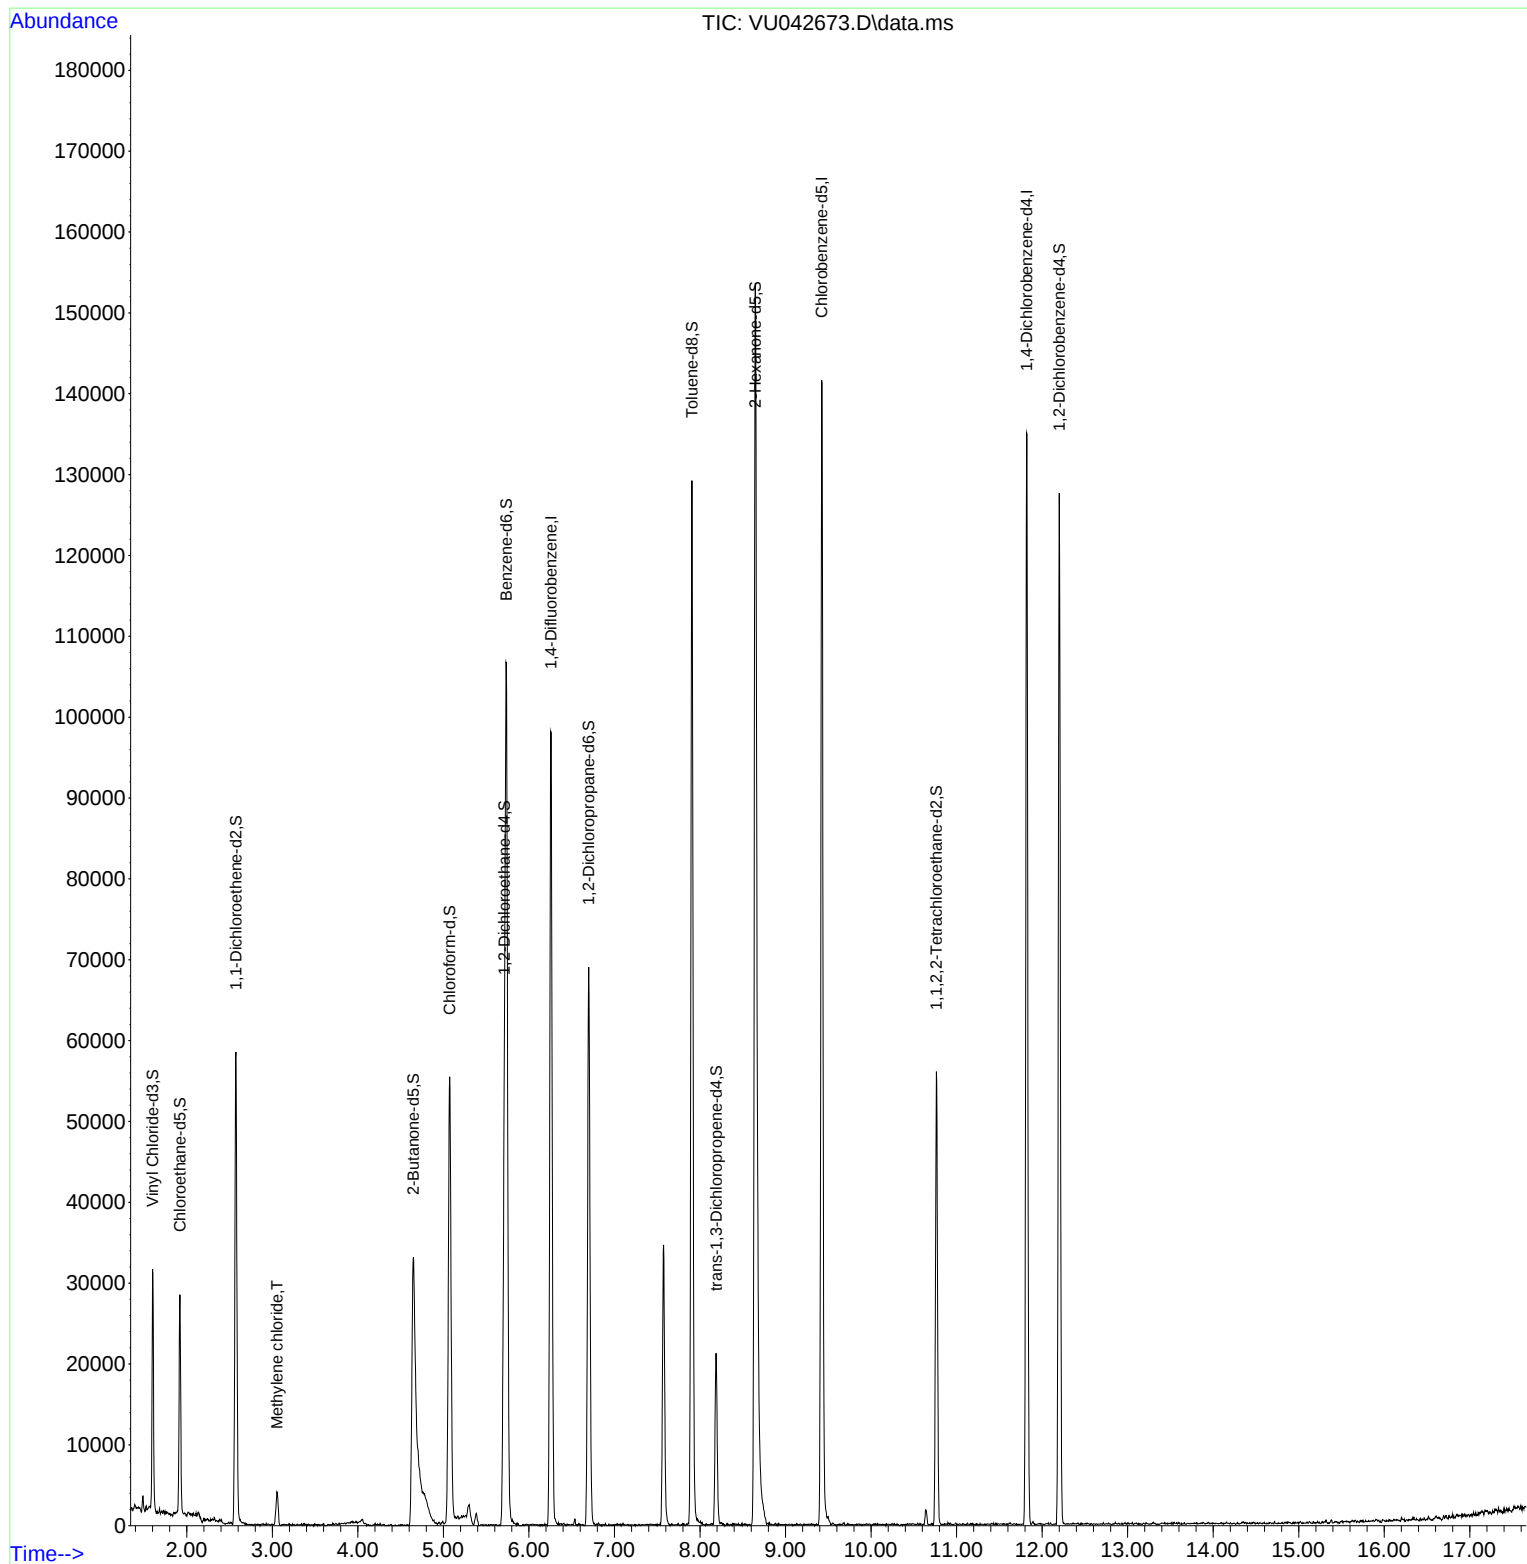

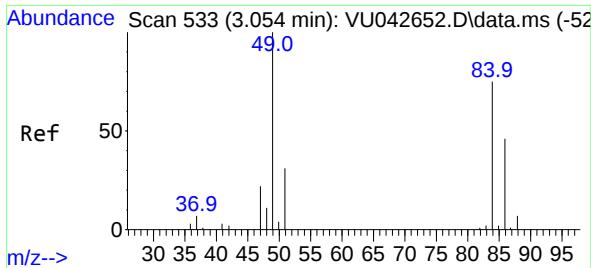

#16
Methylene chloride
Concen: 0.28 ug/L
RT: 3.054 min Scan# 533
Delta R.T. -0.000 min
Lab File: VU042673.D
Acq: 15 Mar 2021 18:56

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Tgt Ion: 84 Resp: 1773

Ion	Ratio	Lower	Upper
84	100		
86	66.0	44.1	81.9
49	131.9	95.0	176.4

