
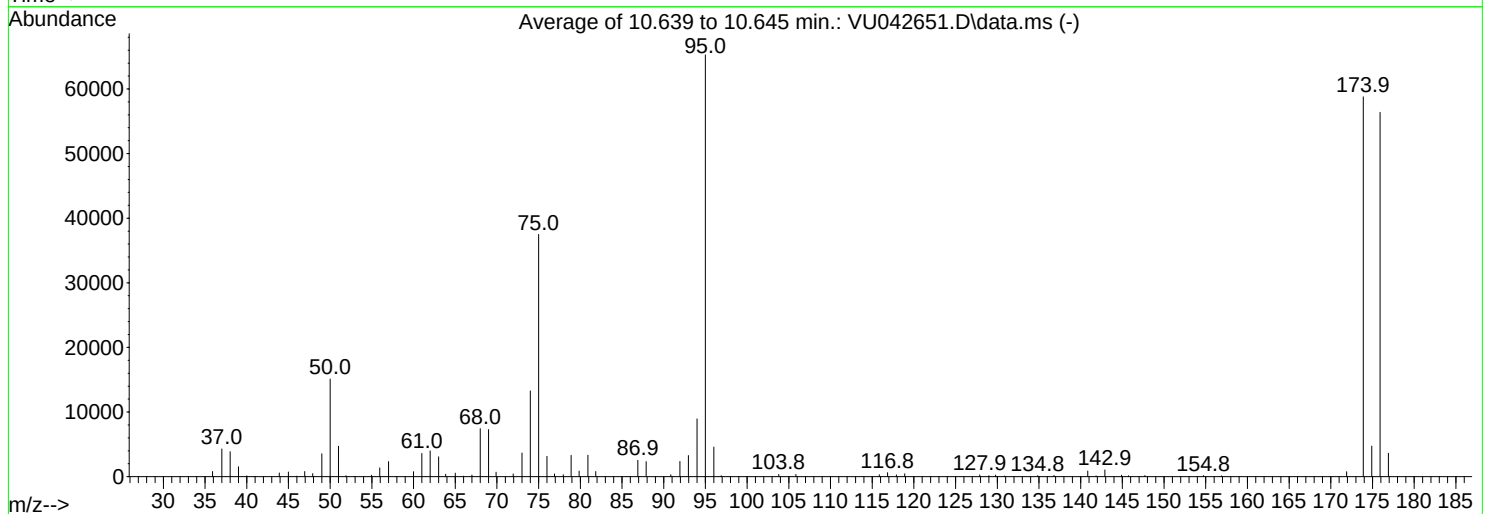


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031521\
Data File : VU042651.D
Acq On : 15 Mar 2021 09:01
Operator : SY/MD
Sample : BFB26
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB26

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Mar 16 01:32:07 2021

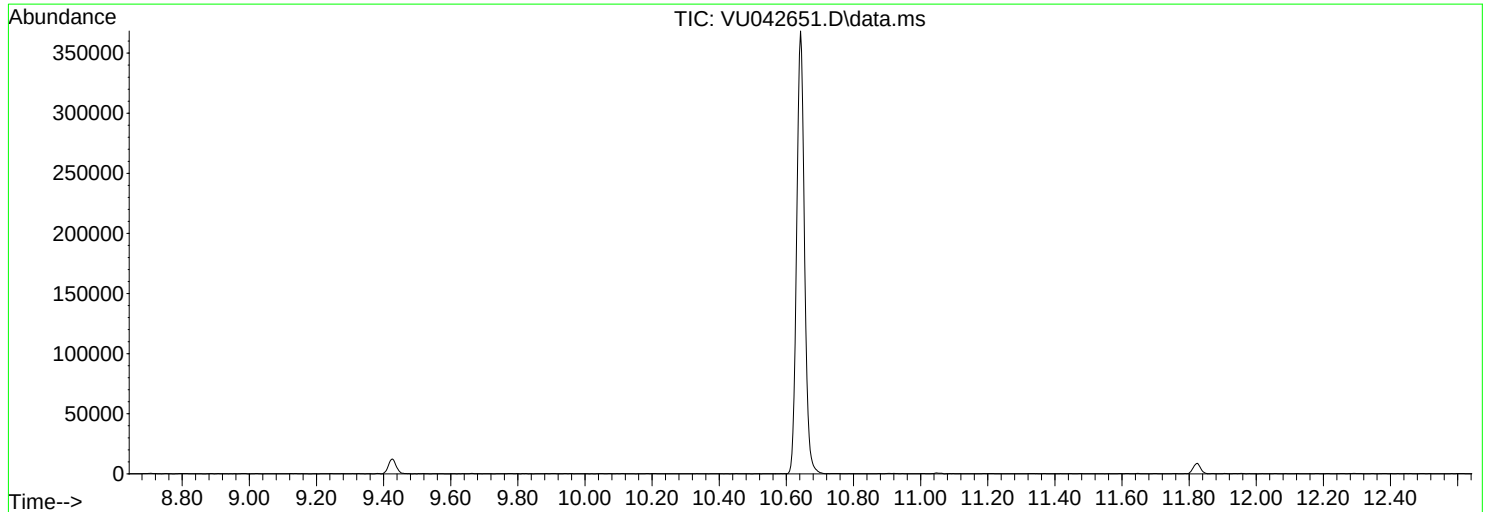

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	15113	PASS
75	95	30	80	57.4	37491	PASS
95	95	100	100	100.0	65285	PASS
96	95	5	9	7.0	4581	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.0	58787	PASS
175	174	5	9	8.1	4737	PASS
176	174	95	101	95.9	56384	PASS
177	176	5	9	6.4	3631	PASS

m/z	Abundance
35.90	875.0
37.00	4088.0
38.00	3909.0
39.00	1631.0
40.00	122.0
40.80	103.0
43.90	689.0
45.00	759.0
45.90	126.0
46.90	732.0
47.90	536.0
49.00	3582.0
50.00	14869.0
51.00	4699.0
51.90	122.0
54.90	269.0
56.00	1357.0
57.00	2446.0
60.00	783.0
61.00	3676.0
62.00	4032.0
63.00	3013.0
63.90	359.0
65.00	492.0
67.00	241.0
68.00	7425.0
69.00	7366.0
69.90	734.0
71.90	422.0
73.00	3585.0
74.00	13353.0
75.00	37104.0
76.00	3080.0
76.90	496.0
77.90	275.0
78.90	3246.0
79.80	818.0
80.90	3330.0
81.90	785.0
86.90	2482.0
87.90	2158.0
90.80	310.0
91.90	2341.0
92.90	3207.0
94.00	8670.0
95.00	63856.0
96.00	4565.0
96.90	171.0
103.80	331.0
105.80	334.0
115.90	300.0
116.80	601.0
117.90	276.0
118.90	428.0
127.90	254.0
129.00	124.0
129.80	249.0
130.80	145.0
134.90	115.0
136.80	222.0
140.90	808.0
141.90	109.0
142.90	1021.0
144.90	208.0
145.70	125.0
147.70	125.0
154.70	158.0
156.90	125.0
171.90	786.0
173.90	56408.0
174.90	4688.0
175.90	53944.0
176.90	3515.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
35.90	828.0
37.00	4424.0
38.00	3979.0
39.00	1565.0
40.00	133.0
43.90	708.0
45.00	754.0
46.00	104.0
47.00	816.0
47.90	479.0
49.00	3673.0
50.00	15563.0
51.00	4843.0
51.90	150.0
52.90	106.0
55.00	233.0
55.90	1459.0
57.00	2398.0
57.90	118.0
60.00	807.0
61.00	3709.0
62.00	4149.0
63.00	3156.0
63.80	363.0
65.00	574.0
66.00	136.0
67.00	253.0
68.00	7622.0
69.00	7421.0
69.90	722.0
71.90	423.0
73.00	3775.0
74.00	13599.0
75.00	38864.0
76.00	3280.0
76.90	418.0
77.90	330.0
78.90	3333.0
79.80	871.0
80.90	3434.0
81.90	823.0
86.90	2574.0
87.90	2395.0
90.90	291.0
92.00	2440.0
93.00	3385.0
94.00	9296.0
95.00	67520.0
96.00	4739.0
96.90	170.0
103.80	370.0
105.90	364.0
115.90	318.0
116.90	652.0
117.90	292.0
118.90	446.0
127.90	287.0
129.00	162.0
129.80	255.0
130.90	130.0
134.90	150.0
136.80	225.0
140.90	885.0
141.90	126.0
142.90	1079.0
144.90	226.0
145.80	156.0
147.70	177.0
154.80	178.0
156.90	125.0
171.90	808.0
173.90	60768.0
174.90	4914.0
175.90	58320.0
176.90	3728.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
35.90	707.0
37.00	4330.0
38.00	3686.0
39.00	1453.0
40.00	144.0
43.90	662.0
45.00	661.0
47.00	854.0
47.90	399.0
49.00	3395.0
50.00	14907.0
51.00	4563.0
51.90	149.0
55.00	208.0
55.90	1290.0
57.00	2138.0
60.00	749.0
61.00	3392.0
62.00	3792.0
63.00	3056.0
63.80	373.0
65.00	566.0
66.00	115.0
67.00	247.0
68.00	7225.0
69.00	7037.0
69.90	625.0
72.00	394.0
73.00	3667.0
74.00	12841.0
75.00	36504.0
76.00	3071.0
76.90	358.0
78.00	311.0
78.90	3280.0
79.90	888.0
80.90	3203.0
81.80	760.0
85.60	114.0
86.90	2538.0
87.90	2437.0
90.90	271.0
92.00	2268.0
93.00	3247.0
94.00	8857.0
95.00	64480.0
96.00	4440.0
96.90	148.0
103.80	370.0
105.90	368.0
115.80	312.0
116.90	621.0
117.90	281.0
118.90	450.0
127.90	262.0
129.00	182.0
129.80	236.0
134.80	164.0
136.80	186.0
140.80	895.0
141.80	135.0
142.90	1053.0
144.90	224.0
145.80	155.0
147.70	193.0
154.80	168.0
156.90	103.0
171.90	703.0
173.90	59184.0
174.90	4610.0
175.90	56888.0
176.90	3650.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
44.00	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26