




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053210.D
 Acq On : 15 Mar 2023 19:00
 Operator : JC/MD
 Sample : 01929-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF0

Manual IntegrationsAPPROVED

Quant Time: Mar 16 04:04:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 16 03:54:54 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

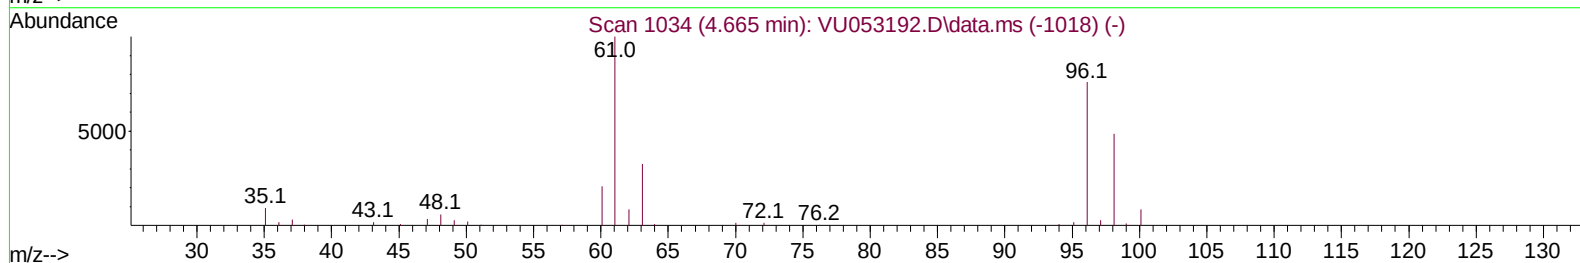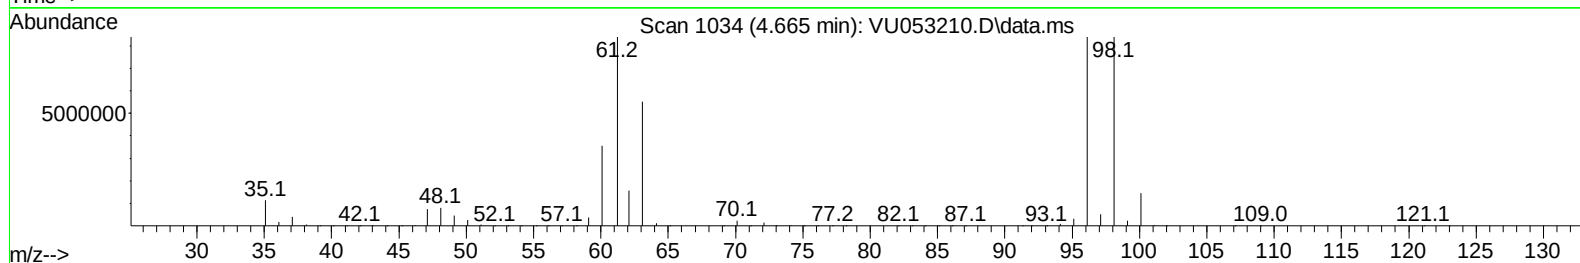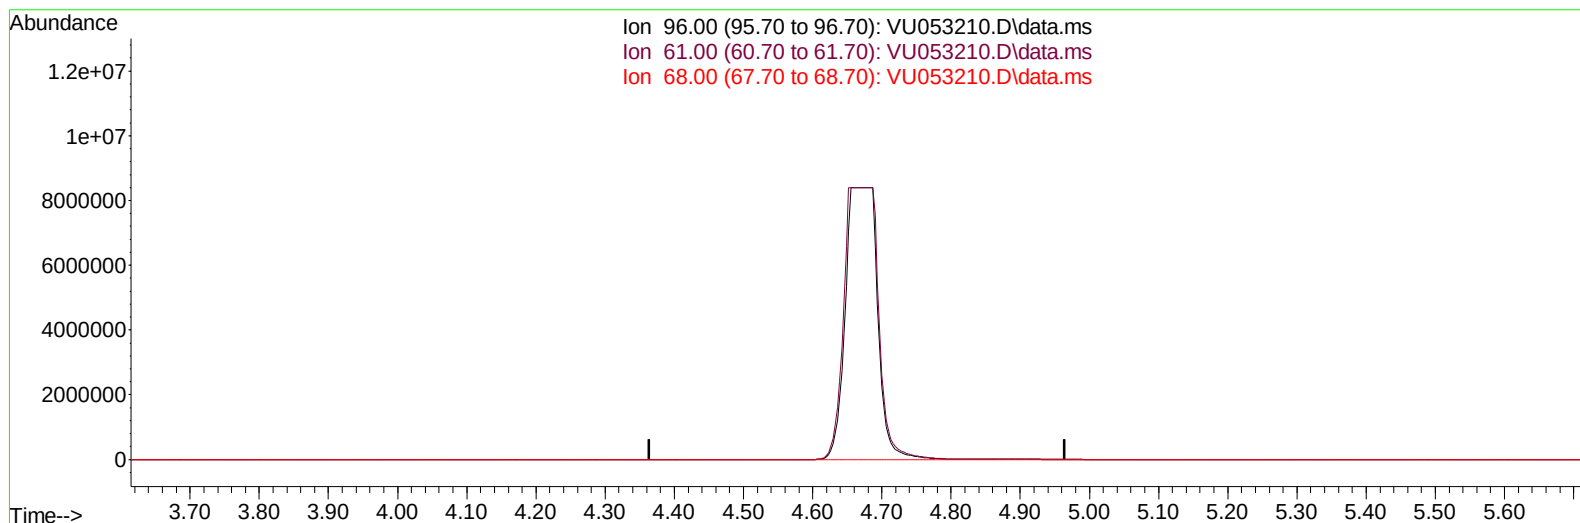

TIC: VU053210.D\data.ms

(20) cis-1,2-Dichloroethene (T)

4.665min (-4.665) 0.00 ug/L

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
61.00	132.10	0.00#
68.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053210.D
 Acq On : 15 Mar 2023 19:00
 Operator : JC/MD
 Sample : 01929-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF0

Manual IntegrationsAPPROVED

Quant Time: Mar 16 04:04:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 16 03:54:54 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

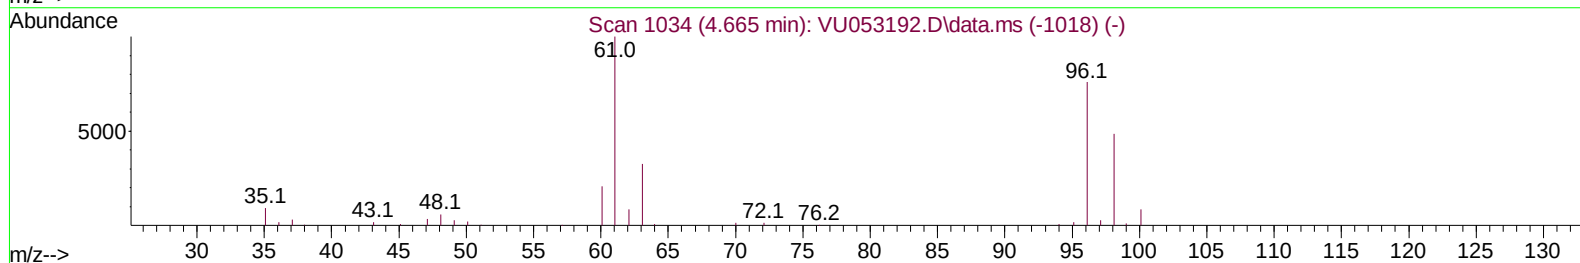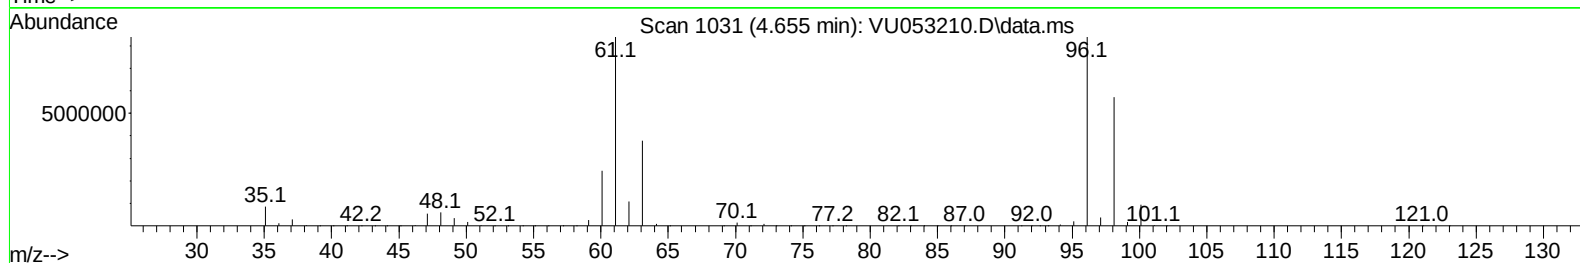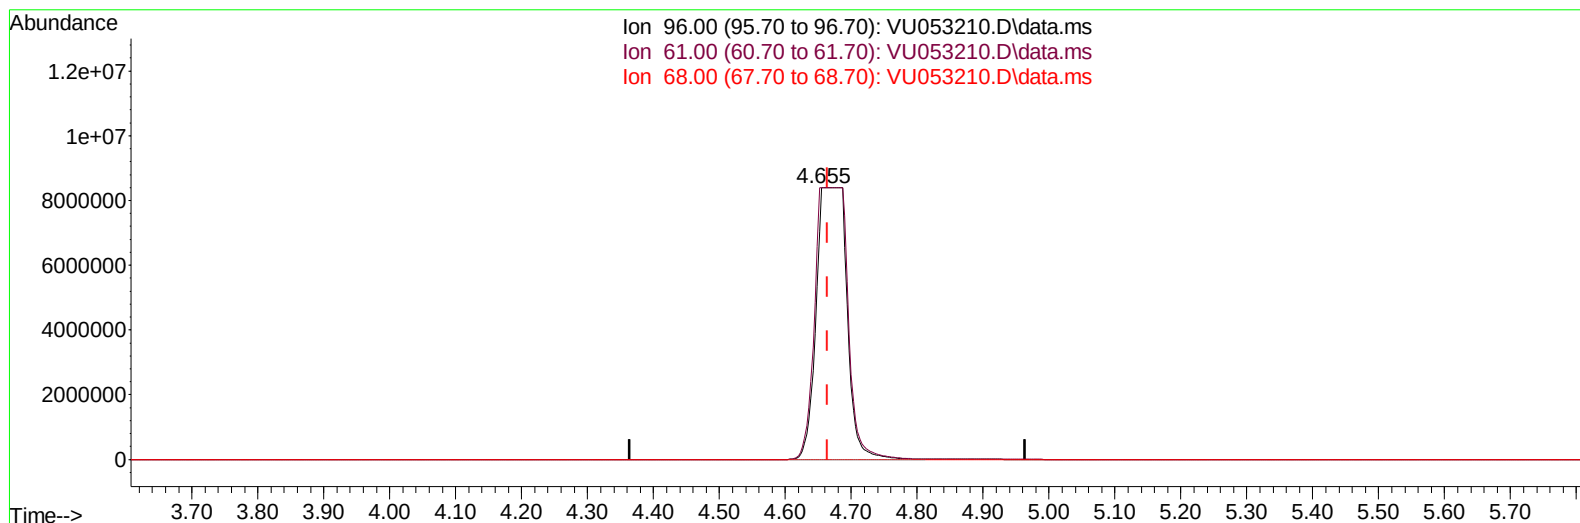

TIC: VU053210.D\data.ms

(20) cis-1,2-Dichloroethene (T)

4.655min (-0.010) 18606.90 ug/L m

response 26961107

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	132.10	100.00
68.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053210.D
 Acq On : 15 Mar 2023 19:00
 Operator : JC/MD
 Sample : 01929-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF0

Manual IntegrationsAPPROVED

Quant Time: Mar 16 04:04:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 16 03:54:54 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

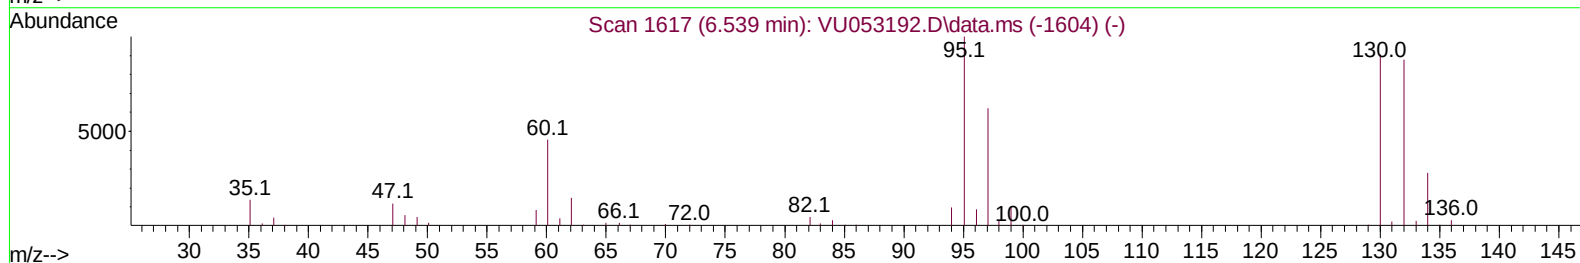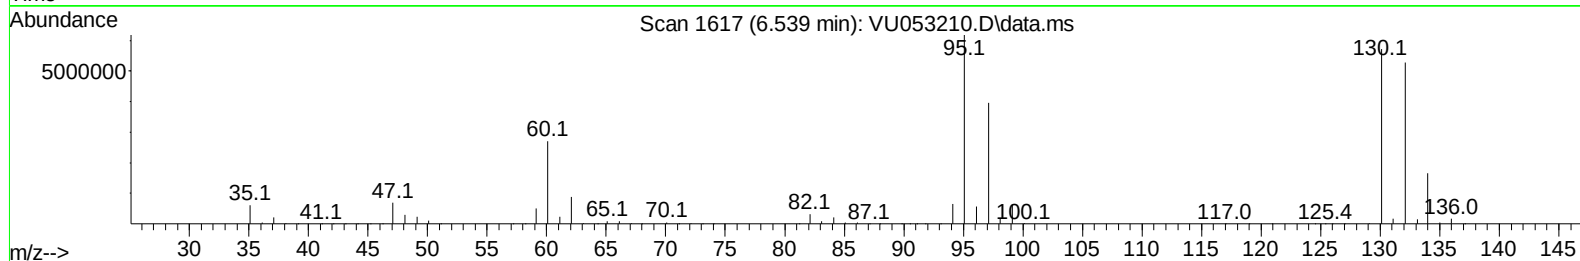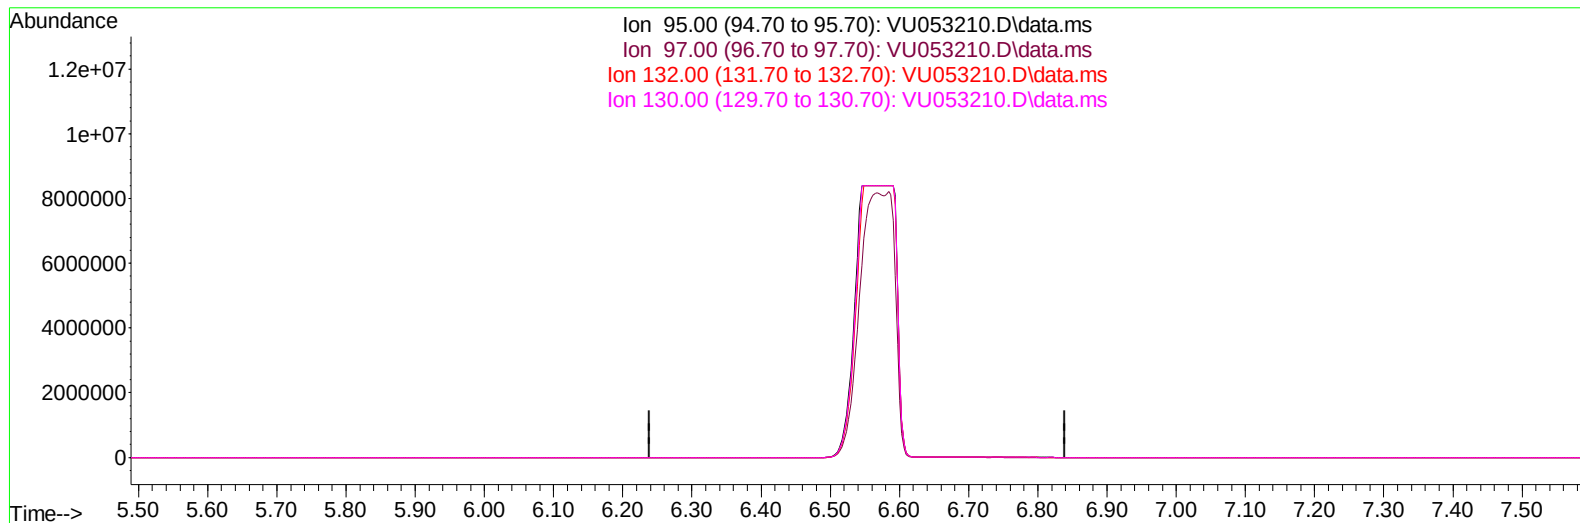

TIC: VU053210.D\data.ms

(34) Trichloroethene (T)

6.539min (-6.539) 0.00 ug/L

response 0

Ion	Exp%	Act%
95.00	100.00	0.00
97.00	62.50	0.00#
132.00	87.90	0.00#
130.00	90.40	0.00#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053210.D
Acq On : 15 Mar 2023 19:00
Operator : JC/MD
Sample : 01929-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF0

Manual IntegrationsAPPROVED

Quant Time: Mar 16 04:04:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 16 03:54:54 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
Supervised By :Mahesh Dadoda 03/17/2023

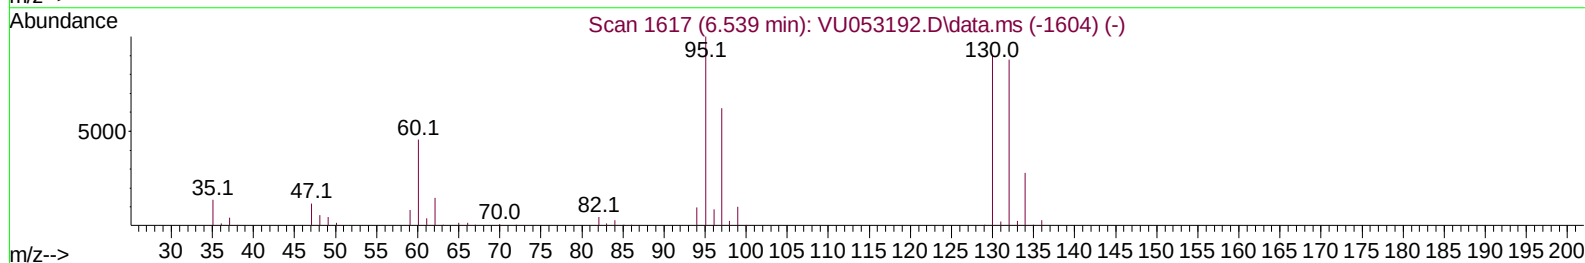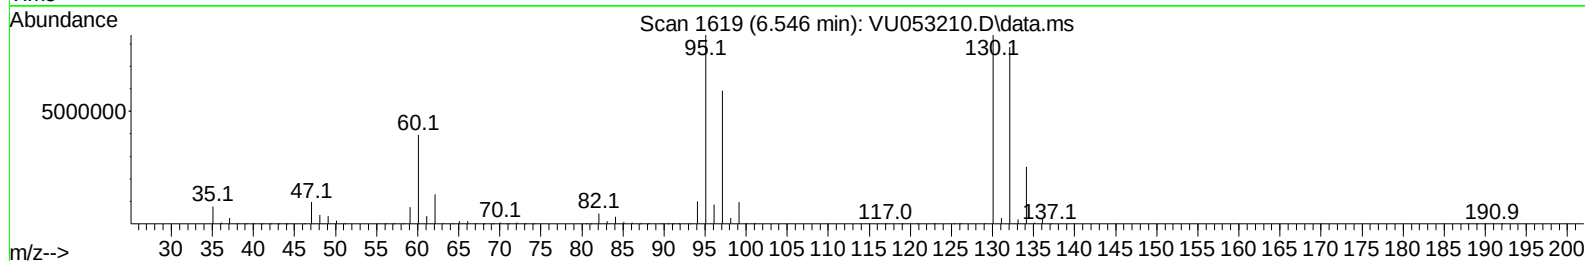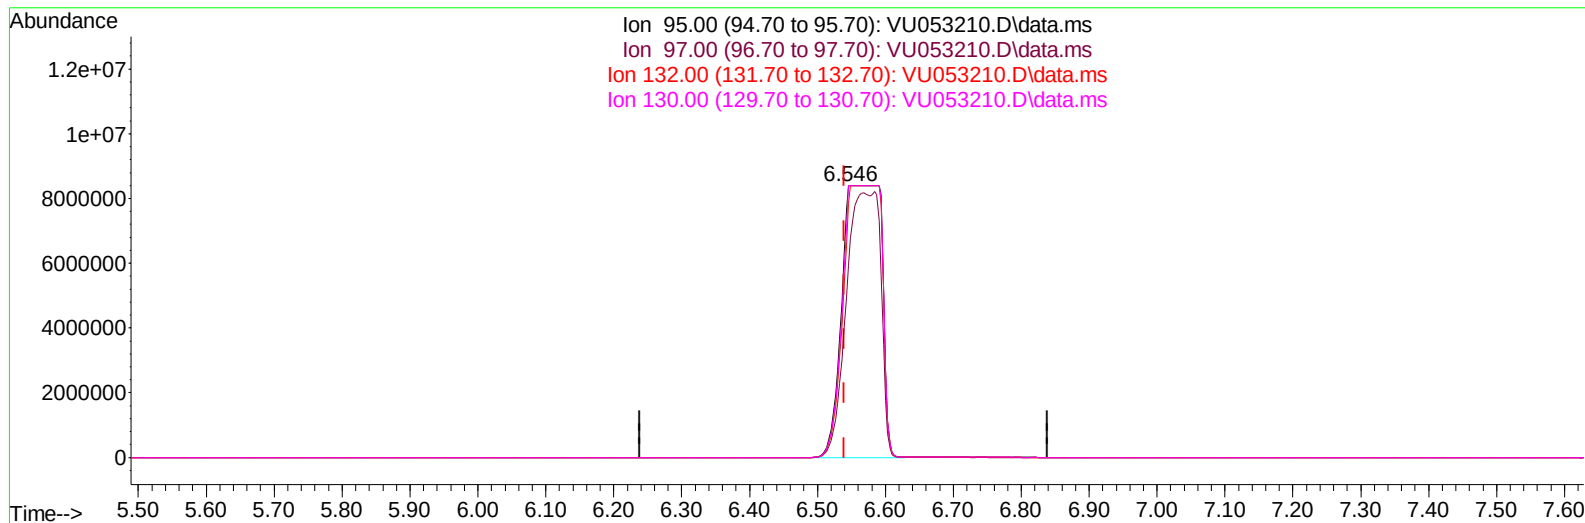

TIC: VU053210.D\data.ms

(34) Trichloroethene (T)

6.546min (+ 0.006) 22698.20 ug/L m

response 33517083

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	62.50	70.63
132.00	87.90	93.51
130.00	90.40	100.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053210.D
 Acq On : 15 Mar 2023 19:00
 Operator : JC/MD
 Sample : 01929-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFF0

Manual IntegrationsAPPROVED

Quant Time: Mar 16 04:04:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 16 03:54:54 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
 Supervised By :Mahesh Dadoda 03/17/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.247	114		165559	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117		163350	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152		83948	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.600	65		94564	61.913	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	123.820%	
7) Chloroethane-d5	1.912	69		55547	44.961	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	89.920%	
11) 1,1-Dichloroethene-d2	2.571	63		117397	44.369	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	88.740%	
21) 2-Butanone-d5	4.661	46		79196	111.795	ug/L	0.04
Spiked Amount 100.000	Range 40	- 130		Recovery	=	111.800%	
24) Chloroform-d	5.060	84		110715	44.010	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	88.020%	
26) 1,2-Dichloroethane-d4	5.697	65		71751	45.925	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	91.860%	
32) Benzene-d6	5.726	84		241049	45.495	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	91.000%	
36) 1,2-Dichloropropane-d6	6.697	67		79401	46.433	ug/L	0.01
Spiked Amount 50.000	Range 70	- 120		Recovery	=	92.860%	
41) Toluene-d8	7.893	98		219552	44.508	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	89.020%	
43) trans-1,3-Dichloroprop...	8.172	79		39282	46.560	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	93.120%	
47) 2-Hexanone-d5	8.629	63		54189	101.362	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	101.360%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84		102433	46.241	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	92.480%	
66) 1,2-Dichlorobenzene-d4	12.188	152		74655	45.928	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	91.860%	
Target Compounds							
						Qvalue	
5) Vinyl chloride	1.604	62	3450505	1980.878	ug/L		99
12) 1,1-Dichloroethene	2.581	96	50820	41.798	ug/L		83
17) trans-1,2-Dichloroethene	3.356	96	165105	133.834	ug/L		99
20) cis-1,2-Dichloroethene	4.655	96	26961107m	18606.901	ug/L		
34) Trichloroethene	6.546	95	33517083m	22698.200	ug/L		
42) Toluene	7.967	91	16029	2.633	ug/L		97
46) Tetrachloroethene	8.552	164	2085	2.170	ug/L		89
70) 1,2,4-trichlorobenzene	13.844	180	2455	1.549	ug/L		91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053210.D
Acq On : 15 Mar 2023 19:00
Operator : JC/MD
Sample : 01929-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFF0

Manual IntegrationsAPPROVED

Quant Time: Mar 16 04:04:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 16 03:54:54 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/16/2023
Supervised By :Mahesh Dadoda 03/17/2023

