

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053205.D
 Acq On : 15 Mar 2023 17:03
 Operator : JC/MD
 Sample : 01929-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE2

Quant Time: Mar 16 04:02:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 16 03:54:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	104403	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	100920	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	52249	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	54357	56.435	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 112.880%		
7) Chloroethane-d5	1.915	69	46046	59.102	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 118.200%		
11) 1,1-Dichloroethene-d2	2.568	63	72873	43.675	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 87.360%		
21) 2-Butanone-d5	4.623	46	56918	127.412	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 127.410%		
24) Chloroform-d	5.057	84	90031	56.751	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 113.500%		
26) 1,2-Dichloroethane-d4	5.697	65	59532	60.425	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 120.840%		
32) Benzene-d6	5.722	84	193983	59.261	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 118.520%		
36) 1,2-Dichloropropane-d6	6.687	67	64362	60.922	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 121.840%#		
41) Toluene-d8	7.893	98	175640	57.632	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 115.260%		
43) trans-1,3-Dichloroprop...	8.176	79	29274	56.162	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 112.320%		
47) 2-Hexanone-d5	8.629	63	42904	129.898	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 129.900%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	81427	59.498	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 119.000%		
66) 1,2-Dichlorobenzene-d4	12.188	152	59694	59.004	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 118.000%		
Target Compounds						
13) Acetone	2.639	43	2601	5.112	ug/L	Qvalue 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053205.D
Acq On : 15 Mar 2023 17:03
Operator : JC/MD
Sample : 01929-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFE2

Quant Time: Mar 16 04:02:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 16 03:54:54 2023
Response via : Initial Calibration

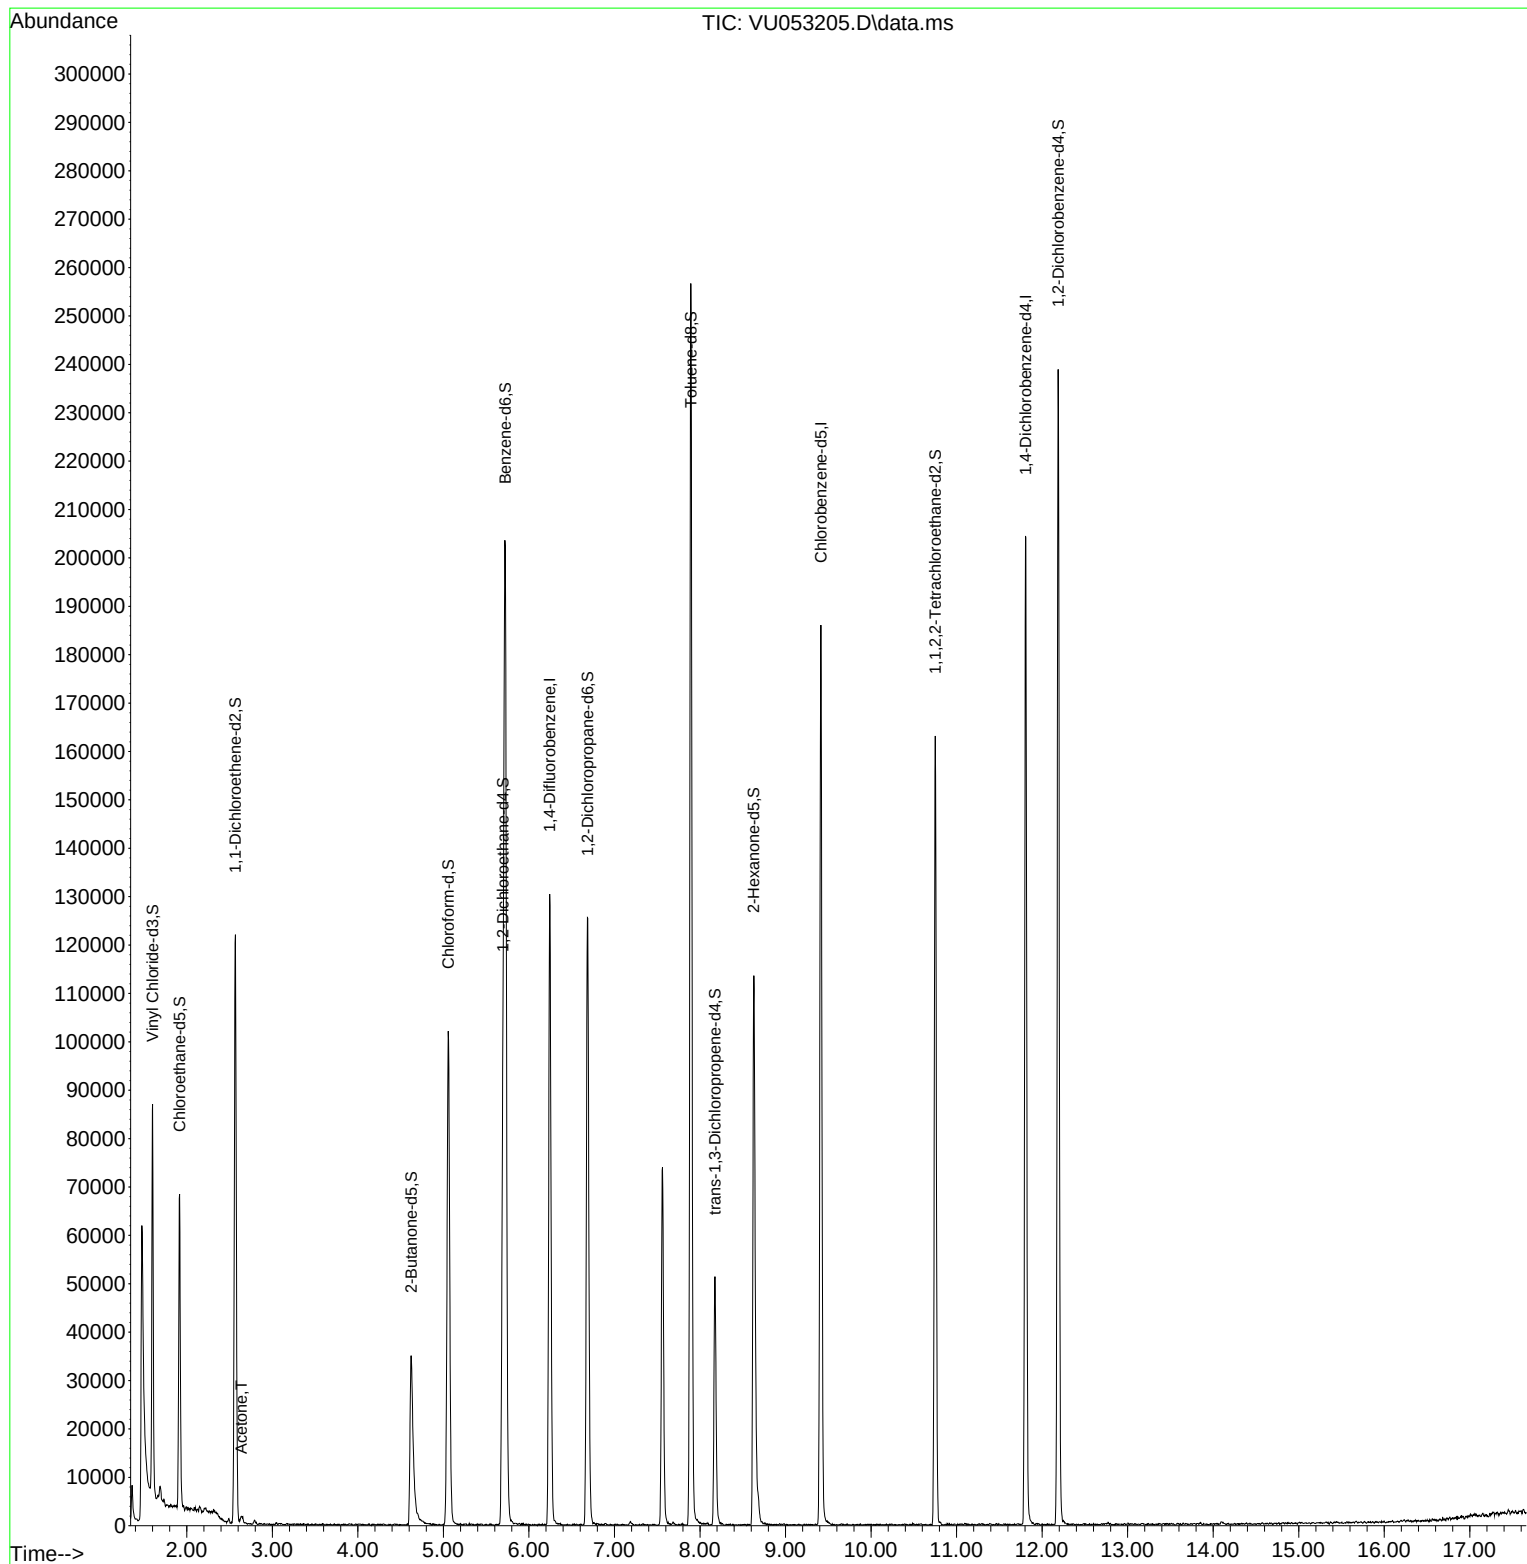

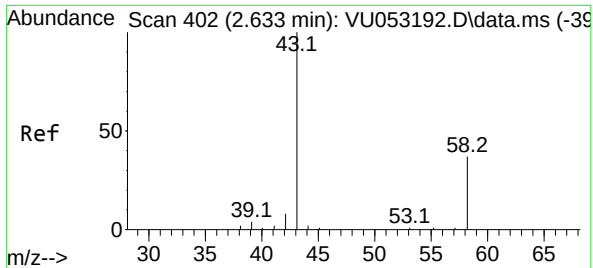

#13
 Acetone
 Concen: 5.112 ug/L
 RT: 2.639 min Scan# 40
 Delta R.T. 0.006 min
 Lab File: VU053205.D
 Acq: 15 Mar 2023 17:03

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFE2

Tgt Ion: 43 Resp: 2601
 Ion Ratio Lower Upper
 43 100
 58 16.6 0.0 75.0

