

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053197.D
 Acq On : 15 Mar 2023 13:57
 Operator : JC/MD
 Sample : 01929-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	98	rVB	103673	118310	16.54%	2.450%
2	1.915	171	179	191	rVB	79715	105407	14.73%	2.182%
3	2.568	369	382	397	rBV	161938	260753	36.45%	5.399%
4	3.462	658	660	661	rBV	203	86	0.01%	0.002%
5	3.497	669	671	674	rVB2	181	103	0.01%	0.002%
6	3.967	814	817	822	rVB	238	116	0.02%	0.002%
7	4.009	827	830	833	rBV2	206	196	0.03%	0.004%
8	4.105	859	860	862	rBV	135	53	0.01%	0.001%
9	4.224	894	897	900	rBV	156	84	0.01%	0.002%
10	4.263	906	909	914	rBV2	209	199	0.03%	0.004%
11	4.465	969	972	975	rBV	160	136	0.02%	0.003%
12	4.542	993	996	1000	rVB	253	163	0.02%	0.003%
13	4.623	1009	1021	1050	rBV	42761	112745	15.76%	2.334%
14	4.877	1097	1100	1102	rBV	303	160	0.02%	0.003%
15	4.938	1118	1119	1120	rBV	123	36	0.01%	0.001%
16	4.983	1130	1133	1134	rBV	141	60	0.01%	0.001%
17	5.057	1140	1156	1177	rBV	130550	287497	40.18%	5.953%
18	5.263	1217	1220	1221	rBV	177	104	0.01%	0.002%
19	5.301	1227	1232	1236	rBV2	233	247	0.03%	0.005%
20	5.443	1273	1276	1281	rBV	245	197	0.03%	0.004%
21	5.468	1281	1284	1286	rBV	192	141	0.02%	0.003%
22	5.539	1305	1306	1308	rBV	133	34	0.00%	0.001%
23	5.719	1342	1362	1386	rBV2	266119	715442	100.00%	14.813%
24	5.967	1434	1439	1444	rBV2	281	265	0.04%	0.005%
25	5.996	1444	1448	1451	rBV2	332	247	0.03%	0.005%
26	6.021	1453	1456	1459	rBV2	257	229	0.03%	0.005%
27	6.144	1492	1494	1495	rBV2	135	59	0.01%	0.001%
28	6.156	1496	1498	1502	rVB2	367	246	0.03%	0.005%
29	6.189	1502	1508	1510	rBV	204	268	0.04%	0.006%
30	6.243	1511	1525	1545	rBV	139136	264016	36.90%	5.466%
31	6.372	1562	1565	1568	rVB	390	241	0.03%	0.005%
32	6.414	1575	1578	1582	rVB	279	152	0.02%	0.003%
33	6.436	1582	1585	1587	rVB	157	63	0.01%	0.001%
34	6.517	1608	1610	1611	rBV	467	180	0.03%	0.004%
35	6.613	1637	1640	1641	rBV	123	55	0.01%	0.001%
36	6.687	1649	1663	1682	rBV2	161298	315224	44.06%	6.527%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053197.D
 Acq On : 15 Mar 2023 13:57
 Operator : JC/MD
 Sample : 01929-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.806	1698	1700	1703	rVB	430	259	0.04%	0.005%
38	6.825	1703	1706	1711	rBV2	347	264	0.04%	0.005%
39	6.899	1723	1729	1731	rBV	192	241	0.03%	0.005%
40	6.912	1731	1733	1736	rVB	241	127	0.02%	0.003%
41	6.957	1744	1747	1748	rBV	168	79	0.01%	0.002%
42	7.005	1760	1762	1765	rVB	187	79	0.01%	0.002%
43	7.089	1785	1788	1790	rBV	184	116	0.02%	0.002%
44	7.134	1798	1802	1805	rBV2	175	171	0.02%	0.004%
45	7.182	1814	1817	1823	rBV3	572	622	0.09%	0.013%
46	7.253	1836	1839	1842	rVB	195	107	0.01%	0.002%
47	7.295	1850	1852	1856	rVB2	165	89	0.01%	0.002%
48	7.311	1856	1857	1858	rBV2	97	19	0.00%	0.000%
49	7.346	1865	1868	1870	rBV2	169	106	0.01%	0.002%
50	7.388	1879	1881	1883	rBV	147	55	0.01%	0.001%
51	7.562	1921	1935	1951	rBV2	95322	171241	23.93%	3.546%
52	7.771	1998	2000	2001	rBV	105	23	0.00%	0.000%
53	7.793	2001	2007	2010	rBV3	349	432	0.06%	0.009%
54	7.893	2025	2038	2060	rBV	336806	583130	81.51%	12.074%
55	8.115	2104	2107	2109	rBV2	229	136	0.02%	0.003%
56	8.176	2114	2126	2150	rVV	65312	111642	15.60%	2.312%
57	8.324	2169	2172	2175	rBV2	298	200	0.03%	0.004%
58	8.391	2190	2193	2196	rVB	263	172	0.02%	0.004%
59	8.491	2222	2224	2225	rBV	222	96	0.01%	0.002%
60	8.629	2256	2267	2294	rBV2	134443	266115	37.20%	5.510%
61	8.918	2354	2357	2366	rVB2	215	226	0.03%	0.005%
62	9.153	2427	2430	2433	rBV	161	82	0.01%	0.002%
63	9.195	2441	2443	2445	rBV	132	56	0.01%	0.001%
64	9.320	2481	2482	2483	rBV	118	36	0.01%	0.001%
65	9.414	2499	2511	2532	rBV	200627	333627	46.63%	6.908%
66	9.568	2554	2559	2561	rBV2	416	344	0.05%	0.007%
67	9.639	2579	2581	2585	rVB	305	139	0.02%	0.003%
68	9.758	2615	2618	2621	rBV2	183	137	0.02%	0.003%
69	9.777	2621	2624	2628	rVB	220	108	0.02%	0.002%
70	9.941	2672	2675	2678	rBV	170	113	0.02%	0.002%
71	10.307	2786	2789	2793	rBV	193	147	0.02%	0.003%
72	10.568	2867	2870	2873	rBV2	176	109	0.02%	0.002%
73	10.751	2915	2927	2947	rBV	202832	322151	45.03%	6.670%
74	11.018	3006	3010	3012	rBV	238	167	0.02%	0.003%
75	11.092	3025	3033	3036	rBV4	647	861	0.12%	0.018%
76	11.127	3042	3044	3045	rBV4	232	68	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053197.D
 Acq On : 15 Mar 2023 13:57
 Operator : JC/MD
 Sample : 01929-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.217	3069	3072	3075	rBV	160	101	0.01%	0.002%
78	11.249	3079	3082	3084	rVV	229	140	0.02%	0.003%
79	11.452	3142	3145	3147	rBV2	353	258	0.04%	0.005%
80	11.529	3165	3169	3171	rBV	244	194	0.03%	0.004%
81	11.748	3231	3237	3241	rBV2	965	1058	0.15%	0.022%
82	11.806	3244	3255	3283	rVV	213793	348678	48.74%	7.219%
83	11.979	3307	3309	3312	rBV	214	83	0.01%	0.002%
84	12.188	3362	3374	3397	rBV	293442	486423	67.99%	10.071%
85	12.458	3456	3458	3462	rVB2	224	182	0.03%	0.004%
86	12.992	3621	3624	3630	rBV2	249	302	0.04%	0.006%
87	13.224	3689	3696	3704	rBV4	1496	1943	0.27%	0.040%
88	13.471	3770	3773	3776	rBV	222	126	0.02%	0.003%
89	13.844	3881	3889	3898	rBV5	1996	3092	0.43%	0.064%
90	14.092	3959	3966	3982	rVB3	3435	5377	0.75%	0.111%
91	14.327	4034	4039	4052	rVB5	2886	3939	0.55%	0.082%
92	14.555	4107	4110	4114	rBV2	354	317	0.04%	0.007%
93	14.912	4218	4221	4222	rBV	303	190	0.03%	0.004%




Sum of corrected areas: 4829809

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053197.D
Acq On : 15 Mar 2023 13:57
Operator : JC/MD
Sample : 01929-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

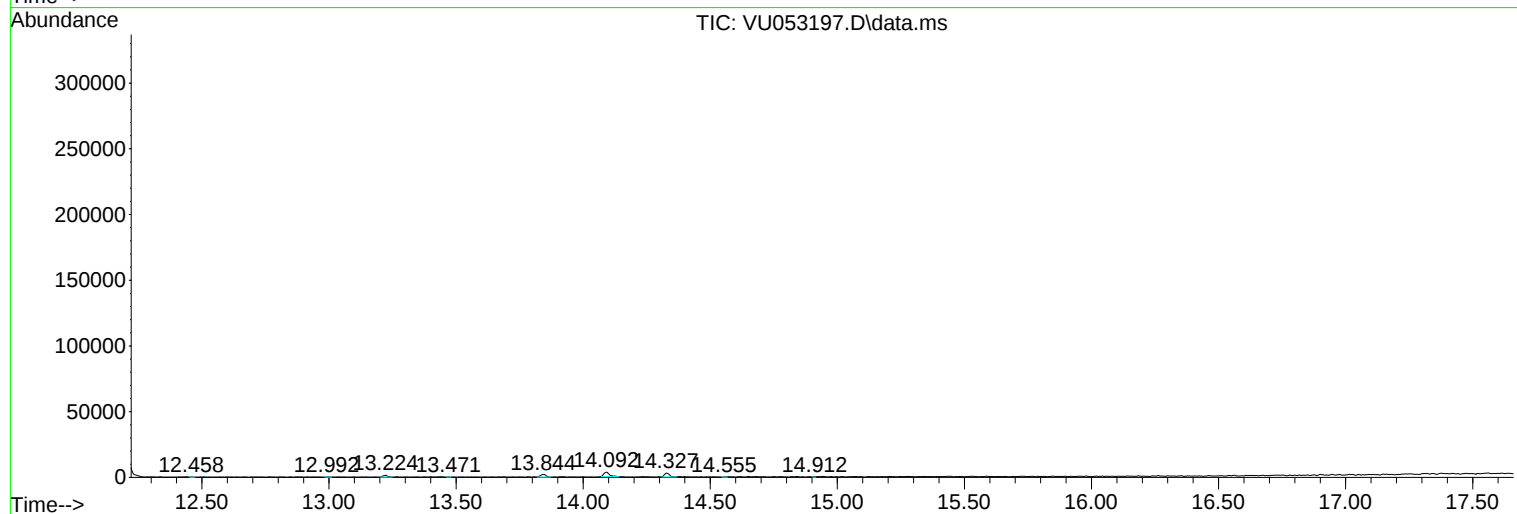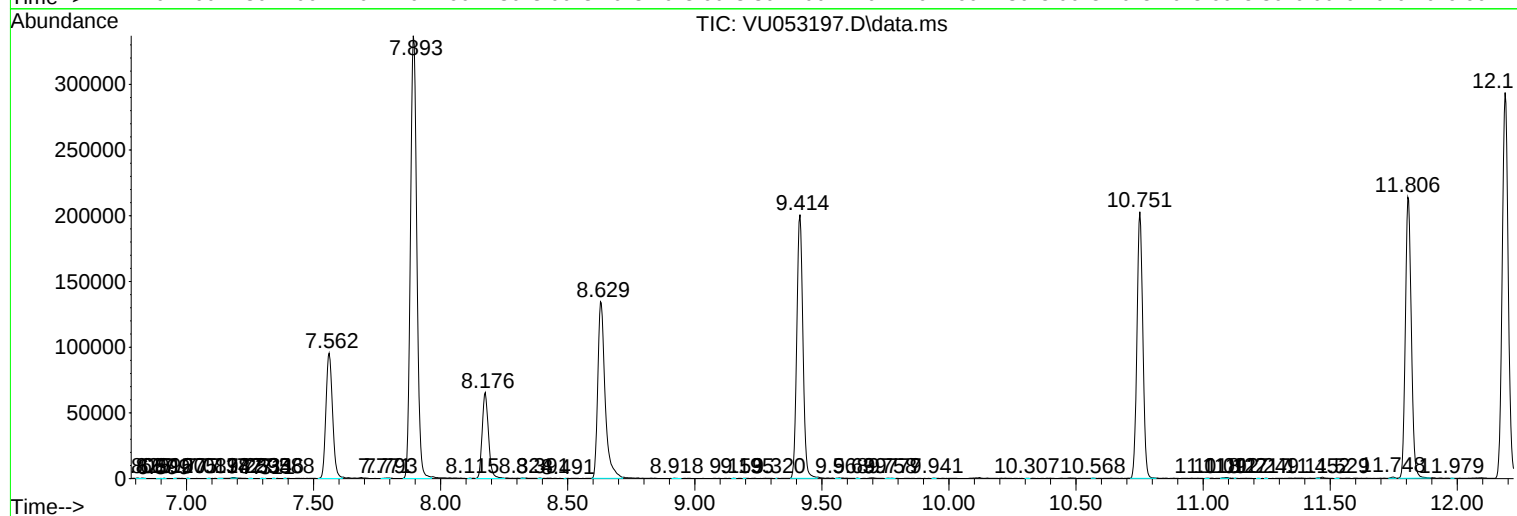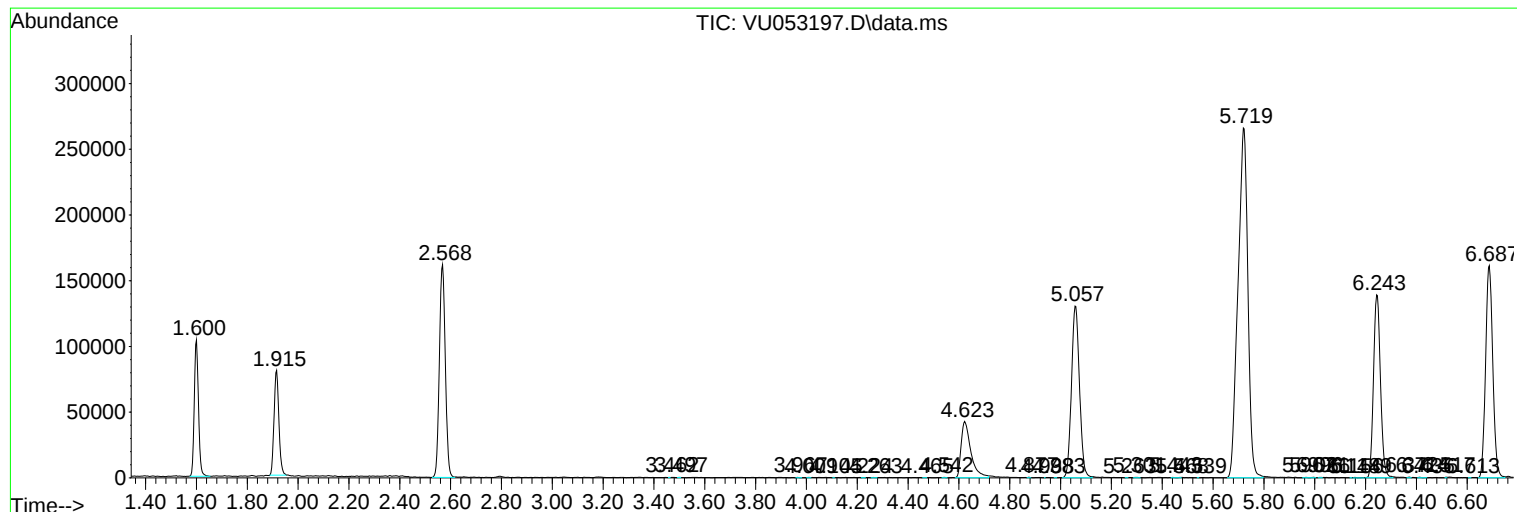

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053197.D
Acq On : 15 Mar 2023 13:57
Operator : JC/MD
Sample : 01929-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053197.D
Acq On : 15 Mar 2023 13:57
Operator : JC/MD
Sample : 01929-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc