

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053198.D
 Acq On : 15 Mar 2023 14:20
 Operator : JC/MD
 Sample : 01929-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	98	rVB	106400	120691	16.82%	2.351%
2	1.916	170	179	195	rBV	80281	106644	14.86%	2.077%
3	2.568	370	382	397	rVB	161492	261957	36.50%	5.102%
4	3.289	603	606	607	rBV	227	162	0.02%	0.003%
5	3.456	655	658	665	rVB2	340	310	0.04%	0.006%
6	3.504	670	673	676	rBV2	178	120	0.02%	0.002%
7	3.768	752	755	758	rBV2	219	145	0.02%	0.003%
8	3.813	767	769	773	rVB2	186	107	0.01%	0.002%
9	3.832	773	775	777	rBV	196	101	0.01%	0.002%
10	3.938	806	808	811	rBV2	198	165	0.02%	0.003%
11	3.973	817	819	820	rBV2	160	77	0.01%	0.001%
12	4.022	831	834	835	rBV	159	71	0.01%	0.001%
13	4.430	959	961	963	rBV2	145	85	0.01%	0.002%
14	4.456	967	969	972	rVB	248	128	0.02%	0.002%
15	4.485	973	978	981	rBV2	288	296	0.04%	0.006%
16	4.623	1009	1021	1047	rBV	42178	119891	16.71%	2.335%
17	4.932	1116	1117	1118	rBV	183	59	0.01%	0.001%
18	5.057	1141	1156	1177	rBV	133417	293575	40.91%	5.718%
19	5.208	1199	1203	1207	rVB2	206	154	0.02%	0.003%
20	5.227	1207	1209	1210	rBV2	139	76	0.01%	0.001%
21	5.263	1217	1220	1223	rBV2	159	148	0.02%	0.003%
22	5.324	1236	1239	1243	rBV2	156	122	0.02%	0.002%
23	5.346	1243	1246	1248	rBV	195	113	0.02%	0.002%
24	5.504	1292	1295	1301	rVB2	395	461	0.06%	0.009%
25	5.543	1301	1307	1312	rBV	342	565	0.08%	0.011%
26	5.568	1313	1315	1318	rVV	237	176	0.02%	0.003%
27	5.584	1318	1320	1322	rVB	194	88	0.01%	0.002%
28	5.723	1341	1363	1395	rBV2	264645	717655	100.00%	13.977%
29	5.890	1412	1415	1420	rBV3	340	416	0.06%	0.008%
30	5.973	1438	1441	1443	rBV2	183	128	0.02%	0.002%
31	6.025	1453	1457	1460	rBV	450	330	0.05%	0.006%
32	6.057	1465	1467	1470	rBV	170	108	0.02%	0.002%
33	6.198	1508	1511	1512	rBV	183	104	0.01%	0.002%
34	6.243	1512	1525	1544	rVV	174475	334202	46.57%	6.509%
35	6.404	1572	1575	1581	rVB3	316	390	0.05%	0.008%
36	6.488	1596	1601	1605	rBV	378	371	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053198.D
 Acq On : 15 Mar 2023 14:20
 Operator : JC/MD
 Sample : 01929-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.523	1605	1612	1614	rBV3	706	786	0.11%	0.015%
38	6.588	1630	1632	1636	rVB2	176	105	0.01%	0.002%
39	6.610	1636	1639	1642	rBV	159	112	0.02%	0.002%
40	6.684	1649	1662	1685	rBV	162885	323588	45.09%	6.302%
41	6.800	1695	1698	1699	rBV	245	140	0.02%	0.003%
42	6.867	1717	1719	1723	rVB2	178	125	0.02%	0.002%
43	6.890	1723	1726	1729	rBV2	217	157	0.02%	0.003%
44	7.022	1764	1767	1770	rBV	147	120	0.02%	0.002%
45	7.182	1812	1817	1824	rBV4	875	1240	0.17%	0.024%
46	7.240	1833	1835	1838	rBV	141	113	0.02%	0.002%
47	7.269	1842	1844	1847	rBV	198	134	0.02%	0.003%
48	7.324	1858	1861	1864	rBV2	167	137	0.02%	0.003%
49	7.362	1871	1873	1875	rVB	267	106	0.01%	0.002%
50	7.382	1876	1879	1881	rBV2	282	211	0.03%	0.004%
51	7.420	1889	1891	1893	rBV	255	153	0.02%	0.003%
52	7.446	1896	1899	1903	rVV2	308	296	0.04%	0.006%
53	7.475	1904	1908	1912	rVV2	269	262	0.04%	0.005%
54	7.497	1912	1915	1918	rVB2	227	156	0.02%	0.003%
55	7.562	1920	1935	1957	rBV	99753	176599	24.61%	3.440%
56	7.787	1999	2005	2006	rBV2	345	316	0.04%	0.006%
57	7.845	2021	2023	2025	rBV2	189	112	0.02%	0.002%
58	7.893	2025	2038	2057	rBV	340890	587274	81.83%	11.438%
59	8.121	2106	2109	2110	rBV	303	212	0.03%	0.004%
60	8.176	2115	2126	2148	rVV	66616	113996	15.88%	2.220%
61	8.279	2156	2158	2159	rVB	234	71	0.01%	0.001%
62	8.301	2160	2165	2168	rBV2	466	351	0.05%	0.007%
63	8.321	2168	2171	2172	rBV	158	104	0.01%	0.002%
64	8.378	2186	2189	2190	rBV2	184	100	0.01%	0.002%
65	8.417	2198	2201	2202	rBV	177	101	0.01%	0.002%
66	8.536	2235	2238	2241	rBV2	289	250	0.03%	0.005%
67	8.565	2241	2247	2251	rVB2	216	338	0.05%	0.007%
68	8.629	2256	2267	2295	rBV2	133092	268215	37.37%	5.224%
69	8.819	2324	2326	2330	rBV2	166	109	0.02%	0.002%
70	8.861	2334	2339	2342	rBV	247	268	0.04%	0.005%
71	8.912	2350	2355	2359	rVB2	221	237	0.03%	0.005%
72	9.128	2418	2422	2423	rBV	186	154	0.02%	0.003%
73	9.231	2451	2454	2458	rBV2	190	184	0.03%	0.004%
74	9.256	2459	2462	2465	rBV2	168	112	0.02%	0.002%
75	9.362	2493	2495	2498	rVB	191	117	0.02%	0.002%
76	9.414	2498	2511	2529	rBV	250552	416413	58.02%	8.110%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
 Data File : VU053198.D
 Acq On : 15 Mar 2023 14:20
 Operator : JC/MD
 Sample : 01929-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYFC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	9.626	2573	2577	2579	rBV2	183	169	0.02%	0.003%
78	9.687	2593	2596	2604	rVB3	390	499	0.07%	0.010%
79	9.735	2608	2611	2612	rBV	156	92	0.01%	0.002%
80	9.787	2625	2627	2628	rBV	172	78	0.01%	0.002%
81	9.845	2642	2645	2648	rBV	257	177	0.02%	0.003%
82	10.105	2721	2726	2730	rBV3	393	446	0.06%	0.009%
83	10.179	2743	2749	2752	rBV2	248	242	0.03%	0.005%
84	10.751	2915	2927	2945	rBV	207728	330639	46.07%	6.440%
85	11.201	3064	3067	3069	rVB	212	97	0.01%	0.002%
86	11.282	3088	3092	3095	rBV	251	211	0.03%	0.004%
87	11.459	3144	3147	3148	rBV2	378	215	0.03%	0.004%
88	11.732	3229	3232	3233	rBV	340	189	0.03%	0.004%
89	11.806	3244	3255	3278	rBV	270331	437410	60.95%	8.519%
90	11.964	3301	3304	3307	rVB	206	99	0.01%	0.002%
91	11.989	3310	3312	3315	rBV2	186	116	0.02%	0.002%
92	12.073	3331	3338	3344	rBV6	1515	2625	0.37%	0.051%
93	12.189	3362	3374	3394	rBV	309873	500379	69.72%	9.746%
94	13.021	3630	3633	3635	rBV	198	96	0.01%	0.002%
95	13.131	3664	3667	3670	rBV	266	171	0.02%	0.003%
96	13.214	3690	3693	3698	rBV4	777	681	0.09%	0.013%
97	13.587	3807	3809	3813	rBV	292	157	0.02%	0.003%
98	13.841	3883	3888	3896	rBV4	1953	2544	0.35%	0.050%
99	14.089	3961	3965	3975	rVB4	2104	2976	0.41%	0.058%
100	14.851	4198	4202	4205	rBV	439	352	0.05%	0.007%




Sum of corrected areas: 5134425

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053198.D
Acq On : 15 Mar 2023 14:20
Operator : JC/MD
Sample : 01929-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

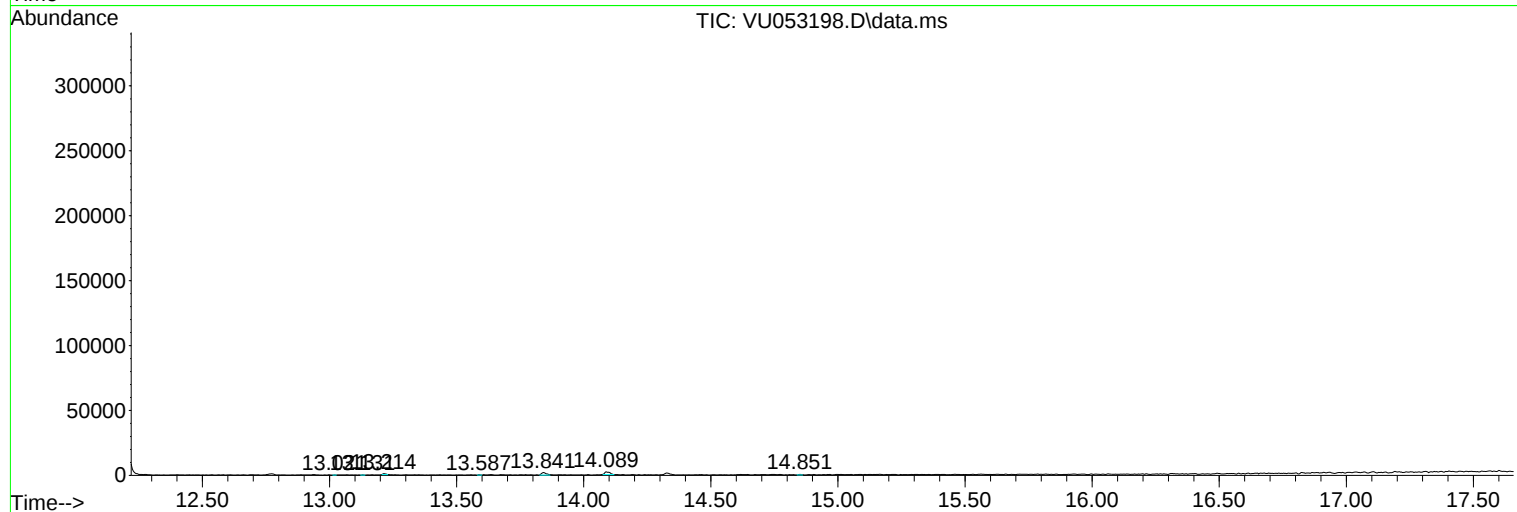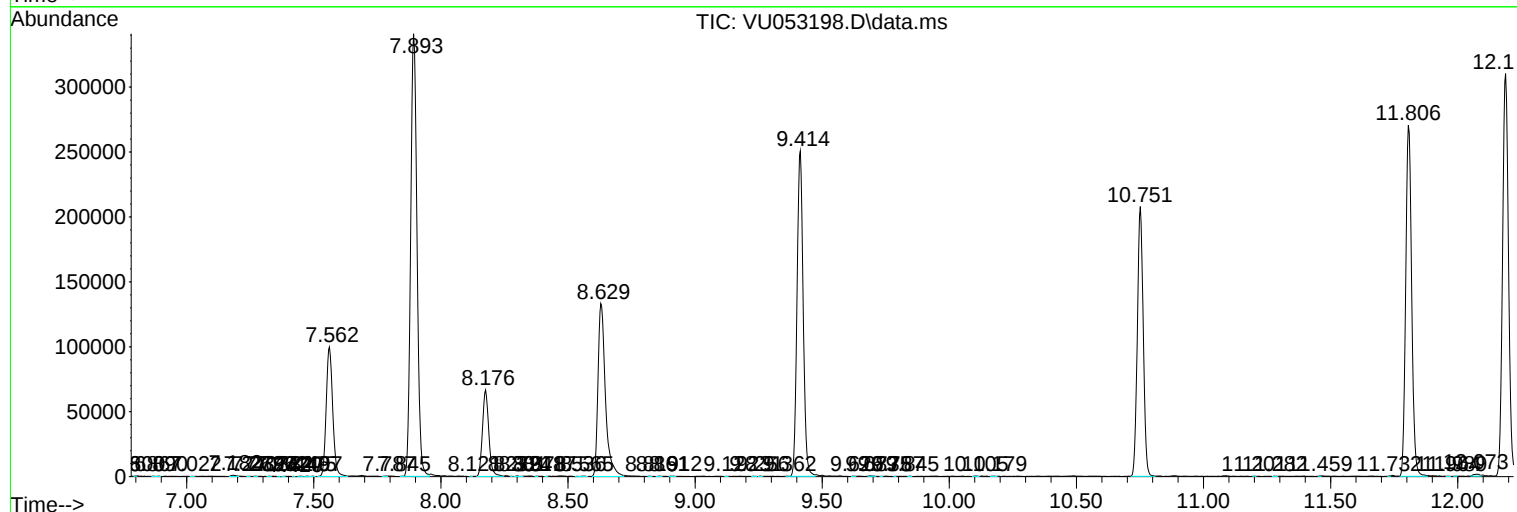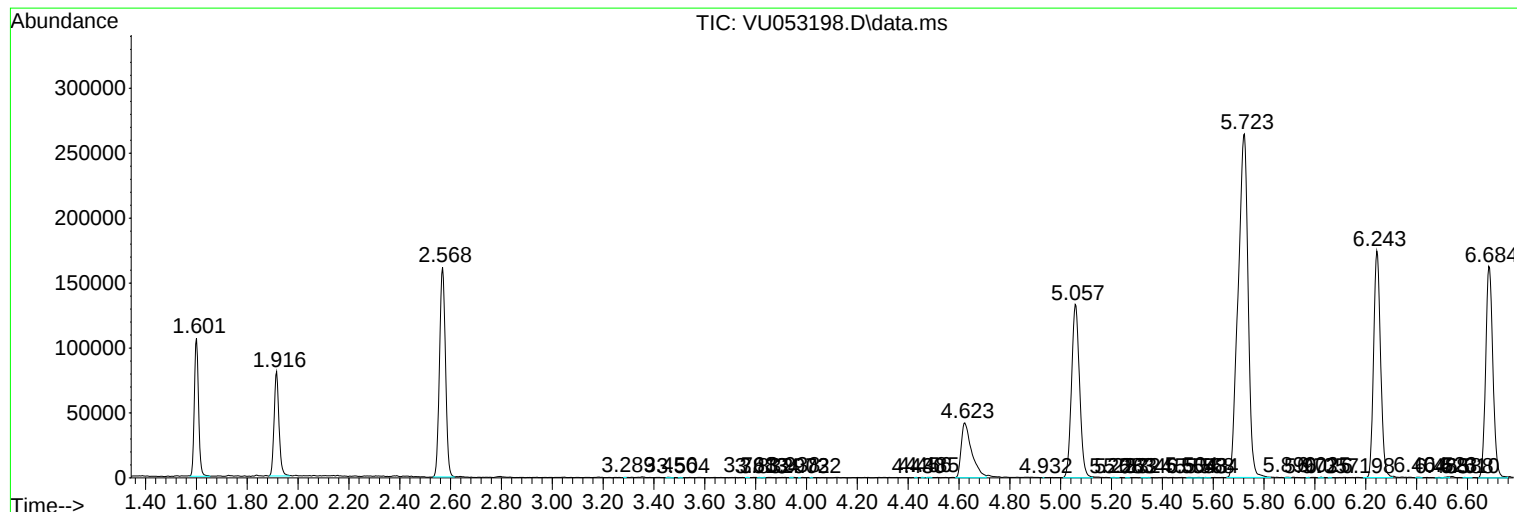

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053198.D
Acq On : 15 Mar 2023 14:20
Operator : JC/MD
Sample : 01929-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU031523\
Data File : VU053198.D
Acq On : 15 Mar 2023 14:20
Operator : JC/MD
Sample : 01929-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYFC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------